AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com
actoolsupply.com

User's manual

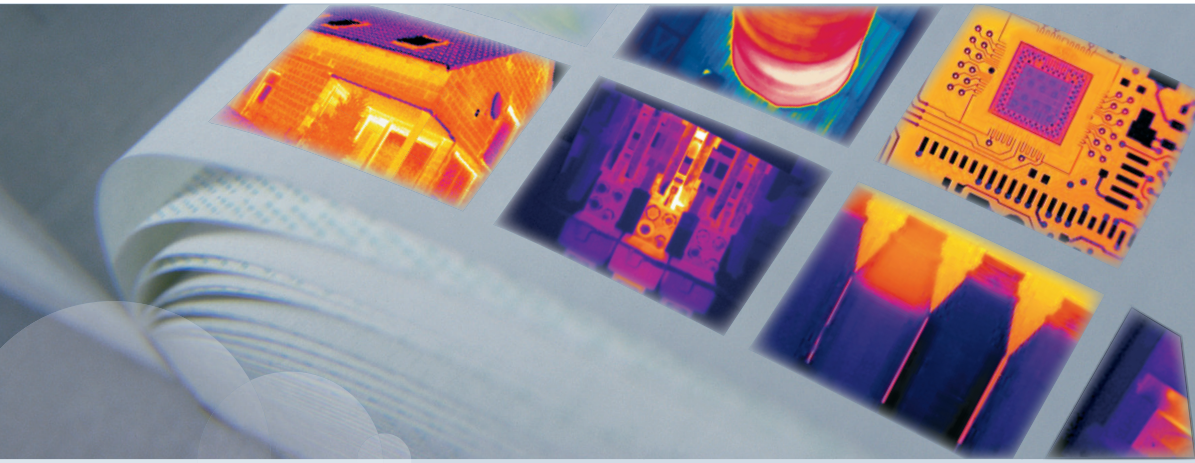

FLIR Txxx series

Publ. No.	T559772
Revision	a593
Language	English (EN)
Issue date	March 16, 2012

actoolsupply.com

Flir T420-NIST Thermal Imaging Infrared Camera Thermography
Flir T440-NIST Thermal Imaging Infrared Camera Thermography
Flir T420-KIT-15 Infrared Camera With 15 Degree Lens
Flir T420-KIT-45 Infrared Camera With 45 Degree Lens
Flir T440-KIT-15 Infrared Camera With 15 Degree Lens
Flir T440-KIT-45 Infrared Camera With 45 Degree Lens
Flir T420bx-NIST Thermal Imaging Infrared Camera Thermography
Flir T440bx-NIST Thermal Imaging Infrared Camera Thermography
Flir T420bx-KIT-15 Infrared Camera With 15 Degree Lens
Flir T420bx-KIT-45 Infrared Camera With 45 Degree Lens
Flir T440bx KIT 15 Infrared Camera With 15 Degree Lens
Flir T440bx KIT 45 Infrared Camera With 45 Degree Lens
FLIR T620 Kit 15 Infrared camera With 15 Degree Lens
FLIR T620 KIT 45 Infrared Camer With 45 Degree Lens
FLIR T620 Thermal Imager With 45 Degree lens
FLIR T620 NIST Thermal Imager With 25 Degree Lens
Flir T640 Infrared Camera With 15 Degree Lens
Flir T640 Infrared Camera With 45 Degree Lens
Flir T640 Infrared Camera With NIST Calibration And 25 Degree Lens
Flir T640 Infrared Camera With NIST Calibration And 15 Degree Lens
Flir T640 Infrared Camera With NIST Calibration And 45 Degree Lens

actoolsupply.com

User's manual

Publ. No. T559772 Rev. a593 – ENGLISH (EN) – March 16, 2012

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

Legal disclaimer

All products manufactured by FLIR Systems are warranted against defective materials and workmanship for a period of one (1) year from the delivery date of the original purchase, provided such products have been under normal storage, use and service, and in accordance with FLIR Systems instruction.

Uncooled handheld infrared cameras manufactured by FLIR Systems are warranted against defective materials and workmanship for a period of two (2) years from the delivery date of the original purchase, provided such products have been under normal storage, use and service, and in accordance with FLIR Systems instruction, and provided that the camera has been registered within 60 days of original purchase.

Detectors for uncooled handheld infrared cameras manufactured by FLIR Systems are warranted against defective materials and workmanship for a period of ten (10) years from the delivery date of the original purchase, provided such products have been under normal storage, use and service, and in accordance with FLIR Systems instruction, and provided that the camera has been registered within 60 days of original purchase.

Products which are not manufactured by FLIR Systems but included in systems delivered by FLIR Systems to the original purchaser, carry the warranty, if any, of the particular supplier only. FLIR Systems has no responsibility whatsoever for such products.

The warranty extends only to the original purchaser and is not transferable. It is not applicable to any product which has been subjected to misuse, neglect, accident or abnormal conditions of operation. Expendable parts are excluded from the warranty.

In the case of a defect in a product covered by this warranty the product must not be further used in order to prevent additional damage. The purchaser shall promptly report any defect to FLIR Systems or this warranty will not apply.

FLIR Systems will, at its option, repair or replace any such defective product free of charge if, upon inspection, it proves to be defective in material or workmanship and provided that it is returned to FLIR Systems within the said one-year period.

FLIR Systems has no other obligation or liability for defects than those set forth above.

No other warranty is expressed or implied. FLIR Systems specifically disclaims the implied warranties of merchantability and fitness for a particular purpose.

FLIR Systems shall not be liable for any direct, indirect, special, incidental or consequential loss or damage, whether based on contract, tort or any other legal theory.

This warranty shall be governed by Swedish law.

Any dispute, controversy or claim arising out of or in connection with this warranty, shall be finally settled by arbitration in accordance with the Rules of the Arbitration Institute of the Stockholm Chamber of Commerce. The place of arbitration shall be Stockholm. The language to be used in the arbitral proceedings shall be English.

Copyright

© 2012, FLIR Systems. All rights reserved worldwide. No parts of the software including source code may be reproduced, transmitted, transcribed or translated into any language or computer language in any form or by any means, electronic, magnetic, optical, manual or otherwise, without the prior written permission of FLIR Systems.

This documentation must not, in whole or part, be copied, photocopied, reproduced, translated or transmitted to any electronic medium or machine readable form without prior consent, in writing, from FLIR Systems.

Names and marks appearing on the products herein are either registered trademarks or trademarks of FLIR Systems and/or its subsidiaries. All other trademarks, trade names or company names referenced herein are used for identification only and are the property of their respective owners.

Quality assurance

The Quality Management System under which these products are developed and manufactured has been certified in accordance with the ISO 9001 standard.

FLIR Systems is committed to a policy of continuous development; therefore we reserve the right to make changes and improvements on any of the products described in this manual without prior notice.

Patents

One or several of the following patents or design patents apply to the products and/or features described in this manual:

0002258-2; 000279476-0001; 000439161; 000499579-0001; 000653423; 000726344; 000859020; 000889290; 001106306-0001; 001707738; 001707746; 001707787; 001776519; 0101577-5; 0102150-0; 0200629-4; 0300911-5; 0302837-0; 1144833; 1182246; 1182620; 1188086; 1285345; 1287138; 1299699; 1325808; 1336775; 1365299; 1402918; 1404291; 1678485; 1732314; 200530018812.0; 200830143636.7; 2106017; 235308; 3006596; 3006597; 466540; 483782; 484155; 518836; 60004227.8; 60122153.2; 602004011681.5-08; 6707044; 68657; 7034300; 7110035; 7154093; 7157705; 7237946; 7312822; 7332716; 7336823; 7544944; 75530; 7667198; 7809258; 7826736; D540838; D549758; D579475; D584755; D599,392; DI6702302-9; DI6703574-4; DI6803572-1; DI6803853-4; DI6903617-9; DM/057692; DM/061609; Registration Number; ZL00809178.1; ZL01823221.3; ZL01823226.4; ZL02331553.9; ZL02331554.7; ZL200480034894.0; ZL200530120994.2; ZL200630130114.4; ZL200730151141.4; ZL200730339504.7; ZL200830128581.2; ZL200930190061.9

EULA Terms

- You have acquired a device (“INFRARED CAMERA”) that includes software licensed by FLIR Systems AB from Microsoft Licensing, GP or its affiliates (“MS”). Those installed software products of MS origin, as well as associated media, printed materials, and “online” or electronic documentation (“SOFTWARE”) are protected by international intellectual property laws and treaties. The SOFTWARE is licensed, not sold. All rights reserved.

actoolsupply.com

actoolsupply.com

- IF YOU DO NOT AGREE TO THIS END USER LICENSE AGREEMENT (“EULA”), DO NOT USE THE DEVICE OR COPY THE SOFTWARE. INSTEAD, PROMPTLY CONTACT FLIR Systems AB FOR INSTRUCTIONS ON RETURN OF THE UNUSED DEVICE(S) FOR A REFUND. **ANY USE OF THE SOFTWARE, INCLUDING BUT NOT LIMITED TO USE ON THE DEVICE, WILL CONSTITUTE YOUR AGREEMENT TO THIS EULA (OR RATIFICATION OF ANY PREVIOUS CONSENT).**
- **GRANT OF SOFTWARE LICENSE.** This EULA grants you the following license:
  - You may use the SOFTWARE only on the DEVICE.
  - **NOT FAULT TOLERANT.** THE SOFTWARE IS NOT FAULT TOLERANT. FLIR Systems AB HAS INDEPENDENTLY DETERMINED HOW TO USE THE SOFTWARE IN THE DEVICE, AND MS HAS RELIED UPON FLIR Systems AB TO CONDUCT SUFFICIENT TESTING TO DETERMINE THAT THE SOFTWARE IS SUITABLE FOR SUCH USE.
  - **NO WARRANTIES FOR THE SOFTWARE.** THE SOFTWARE is provided “AS IS” and with all faults. THE ENTIRE RISK AS TO SATISFACTORY QUALITY, PERFORMANCE, ACCURACY, AND EFFORT (INCLUDING LACK OF NEGLIGENCE) IS WITH YOU. ALSO, THERE IS NO WARRANTY AGAINST INTERFERENCE WITH YOUR ENJOYMENT OF THE SOFTWARE OR AGAINST INFRINGEMENT. **IF YOU HAVE RECEIVED ANY WARRANTIES REGARDING THE DEVICE OR THE SOFTWARE, THOSE WARRANTIES DO NOT ORIGINATE FROM, AND ARE NOT BINDING ON, MS.**
  - No Liability for Certain Damages. **EXCEPT AS PROHIBITED BY LAW, MS SHALL HAVE NO LIABILITY FOR ANY INDIRECT, SPECIAL, CONSEQUENTIAL OR INCIDENTAL DAMAGES ARISING FROM OR IN CONNECTION WITH THE USE OR PERFORMANCE OF THE SOFTWARE. THIS LIMITATION SHALL APPLY EVEN IF ANY REMEDY FAILS OF ITS ESSENTIAL PURPOSE. IN NO EVENT SHALL MS BE LIABLE FOR ANY AMOUNT IN EXCESS OF U.S. TWO HUNDRED FIFTY DOLLARS (U.S.$250.00).**
  - **Limitations on Reverse Engineering, Decompilation, and Disassembly.** You may not reverse engineer, decompile, or disassemble the SOFTWARE, except and only to the extent that such activity is expressly permitted by applicable law notwithstanding this limitation.
  - **SOFTWARE TRANSFER ALLOWED BUT WITH RESTRICTIONS.** You may permanently transfer rights under this EULA only as part of a permanent sale or transfer of the Device, and only if the recipient agrees to this EULA. If the SOFTWARE is an upgrade, any transfer must also include all prior versions of the SOFTWARE.
  - **EXPORT RESTRICTIONS.** You acknowledge that SOFTWARE is subject to U.S. export jurisdiction. You agree to comply with all applicable international and national laws that apply to the SOFTWARE, including the U.S. Export Administration Regulations, as well as end-user, end-use and destination restrictions issued by U.S. and other governments. For additional information see http://www.microsoft.com/exporting/.

Publ. No. T559772 Rev. a593 – ENGLISH (EN) – March 16, 2012

actoolsupply.com

actoolsupply.com

actoolsupply.com

actoolsupply.com

Table of contents

1 Warnings & Cautions 1

2 Notice to user 5

3 Customer help 6

4 Documentation updates 7

5 Important note about this manual 8

6 Quick Start Guide 9

7 Parts lists 10
- 7.1 Contents of the transport case 10
- 7.2 List of accessories 10

8 A note about ergonomics 14

9 Camera parts 15
- 9.1 Rear view 15
- 9.2 Front view 17
- 9.3 Bottom view 19
- 9.4 Battery condition indicator 20
- 9.5 Laser pointer 21

10 Screen elements 23

11 Navigating the menu system 24

12 External devices and storage media 25

13 Pairing Bluetooth devices 26

14 Fetching data from external Extech meters 27
- 14.1 Typical moisture measurement and documentation procedure 29

15 Handling the camera 30
- 15.1 Charging the battery 30
  - 15.1.1 Using the combined power supply and battery charger to charge the battery when it is inside the camera 31
  - 15.1.2 Using the combined power supply and battery charger to charge the battery when it is outside the camera 32
  - 15.1.3 Using the stand-alone battery charger to charge the battery 33
- 15.2 Inserting the battery 34
- 15.3 Removing the battery 36
- 15.4 Turning on and turning off the camera 38
- 15.5 Adjusting the angle of lens 39
- 15.6 Attaching the sunshield 40
- 15.7 Using the laser pointer 42

16 Working with images and folders 43
- 16.1 Adjusting the infrared camera focus 43

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

16.2 Previewing an image ... 44
16.3 Saving an image ... 45
16.4 Periodically saving an image ... 46
16.5 Opening an image ... 47
16.6 Adjusting an image manually ... 48
16.7 Hiding overlay graphics ... 51
16.8 Deleting images ... 52
16.9 Creating an Adobe PDF report ... 53

17 Working with fusion ... 54

18 Recording video clips ... 57

19 Working with measurement tools and isotherms ... 58
19.1 Setting up measurement tools ... 58
19.2 Setting up a difference calculation ... 59
19.3 Setting up isotherms ... 60
19.4 Removing measurement tools ... 63
19.5 Moving measurement tools ... 64
19.6 Resizing areas ... 65
19.7 Changing object parameters ... 66

20 Annotating images ... 68
20.1 Adding a digital photo automatically ... 69
20.2 Adding a digital photo manually ... 70
20.3 Adding a voice annotation ... 71
20.4 Adding a table ... 72
20.5 Adding an text ... 74
20.6 Adding a sketch ... 75

21 Changing settings ... 76
21.1 Changing camera settings ... 76
21.2 Changing preferences ... 77
21.3 Changing connectivity ... 78
21.4 Changing regional settings ... 79

22 Cleaning the camera ... 80
22.1 Camera housing, cables, and other items ... 80
22.2 Infrared lens ... 81
22.3 Infrared detector ... 82

23 Technical data ... 83

24 Pin configurations ... 84

25 Application examples ... 88
25.1 Moisture & water damage ... 88
25.2 Faulty contact in socket ... 89
25.3 Oxidized socket ... 90
25.4 Insulation deficiencies ... 91
25.5 Draft ... 92

26 About FLIR Systems ... 93
26.1 More than just an infrared camera ... 94
26.2 Sharing our knowledge ... 95

actoolsupply.com

actoolsupply.com

26.3 Supporting our customers 95
26.4 A few images from our facilities 95

27 Glossary 97

28 Thermographic measurement techniques 101
28.1 Introduction 101
28.2 Emissivity 101
28.2.1 Finding the emissivity of a sample 102
28.2.1.1 Step 1: Determining reflected apparent temperature 102
28.2.1.2 Step 2: Determining the emissivity 104
28.3 Reflected apparent temperature 105
28.4 Distance 105
28.5 Relative humidity 105
28.6 Other parameters 105

29 History of infrared technology 106

30 Theory of thermography 110
30.1 Introduction 110
30.2 The electromagnetic spectrum 110
30.3 Blackbody radiation 111
30.3.1 Planck's law 112
30.3.2 Wien's displacement law 113
30.3.3 Stefan-Boltzmann's law 115
30.3.4 Non-blackbody emitters 116
30.4 Infrared semi-transparent materials 118

31 The measurement formula 120

32 Emissivity tables 126
32.1 References 126
32.2 Important note about the emissivity tables 126
32.3 Tables 127

actoolsupply.com

actoolsupply.com

actoolsupply.com

actoolsupply.com

1 Warnings & Cautions

WARNING

- (Applies only to Class A digital devices.) This equipment generates, uses, and can radiate radio frequency energy and if not installed and used in accordance with the instruction manual, may cause interference to radio communications. It has been tested and found to comply with the limits for a Class A computing device pursuant to Subpart J of Part 15 of FCC Rules, which are designed to provide reasonable protection against such interference when operated in a commercial environment. Operation of this equipment in a residential area is likely to cause interference in which case the user at his own expense will be required to take whatever measures may be required to correct the interference.
- (Applies only to Class B digital devices.) This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:
  - Reorient or relocate the receiving antenna.
  - Increase the separation between the equipment and receiver.
  - Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
  - Consult the dealer or an experienced radio/TV technician for help.
- (Applies only to digital devices subject to 15.19/RSS-210.) **NOTICE**: This device complies with Part 15 of the FCC Rules and with RSS-210 of Industry Canada. Operation is subject to the following two conditions:

  1 this device may not cause harmful interference, and
  2 this device must accept any interference received, including interference that may cause undesired operation.
- (Applies only to digital devices subject to 15.21.) **NOTICE**: Changes or modifications made to this equipment not expressly approved by (manufacturer name) may void the FCC authorization to operate this equipment.
- (Applies only to digital devices subject to 2.1091/2.1093/OET Bulletin 65.) **Radiofrequency radiation exposure Information**: The radiated output power of the device is far below the FCC radio frequency exposure limits. Nevertheless, the device shall be used in such a manner that the potential for human contact during normal operation is minimized.
- (Applies only to cameras with laser pointer:) Do not look directly into the laser beam. The laser beam can cause eye irritation.
- Applies only to cameras with battery:
  - Do not disassemble or do a modification to the battery. The battery contains safety and protection devices which, if they become damaged, can cause the battery to become hot, or cause an explosion or an ignition.

actoolsupply.com

actoolsupply.com

AC Tool Supply.com 877-207-1244 aikencolon.com

- If there is a leak from the battery and the fluid gets into your eyes, do not rub your eyes. Flush well with water and immediately get medical care. The battery fluid can cause injury to your eyes if you do not do this.
- Do not continue to charge the battery if it does not become charged in the specified charging time. If you continue to charge the battery, it can become hot and cause an explosion or ignition.
- Only use the correct equipment to discharge the battery. If you do not use the correct equipment, you can decrease the performance or the life cycle of the battery. If you do not use the correct equipment, an incorrect flow of current to the battery can occur. This can cause the battery to become hot, or cause an explosion and injury to persons.

- Make sure that you read all applicable MSDS (Material Safety Data Sheets) and warning labels on containers before you use a liquid: the liquids can be dangerous.
- If mounting the A3xx pt/A3xx f series camera on a pole, tower or any elevated location, use industry standard safe practices to avoid injuries.

CAUTION

- Do not point the infrared camera (with or without the lens cover) at intensive energy sources, for example devices that emit laser radiation, or the sun. This can have an unwanted effect on the accuracy of the camera. It can also cause damage to the detector in the camera.
- Do not use the camera in a temperature higher than +50°C (+122°F), unless specified otherwise in the user documentation. High temperatures can cause damage to the camera.
- (Applies only to cameras with laser pointer:) Protect the laser pointer with the protective cap when you do not operate the laser pointer.
- Applies only to cameras with battery:
  - Do not attach the batteries directly to a car's cigarette lighter socket, unless a specific adapter for connecting the batteries to a cigarette lighter socket is provided by FLIR Systems.
  - Do not connect the positive terminal and the negative terminal of the battery to each other with a metal object (such as wire).
  - Do not get water or salt water on the battery, or permit the battery to get wet.
  - Do not make holes in the battery with objects. Do not hit the battery with a hammer. Do not step on the battery, or apply strong impacts or shocks to it.
  - Do not put the batteries in or near a fire, or into direct sunlight. When the battery becomes hot, the built-in safety equipment becomes energized and can stop the battery charging process. If the battery becomes hot, damage can occur to the safety equipment and this can cause more heat, damage or ignition of the battery.
  - Do not put the battery on a fire or increase the temperature of the battery with heat.
  - Do not put the battery on or near fires, stoves, or other high-temperature locations.
  - Do not solder directly onto the battery.
  - Do not use the battery if, when you use, charge, or store the battery, there is an unusual smell from the battery, the battery feels hot, changes color, changes shape, or is in an unusual condition. Contact your sales office if one or more of these problems occurs.
  - Only use a specified battery charger when you charge the battery.

actoolsupply.com

actoolsupply.com

- The temperature range through which you can charge the battery is ±0°C to +45°C (+32°F to +113°F), unless specified otherwise in the user documentation. If you charge the battery at temperatures out of this range, it can cause the battery to become hot or to break. It can also decrease the performance or the life cycle of the battery.
- The temperature range through which you can discharge the battery is −15°C to +50°C (+5°F to +122°F), unless specified otherwise in the user documentation. Use of the battery out of this temperature range can decrease the performance or the life cycle of the battery.
- When the battery is worn, apply insulation to the terminals with adhesive tape or similar materials before you discard it.
- Remove any water or moisture on the battery before you install it.

- Do not apply solvents or similar liquids to the camera, the cables, or other items. This can cause damage.
- Be careful when you clean the infrared lens. The lens has a delicate anti-reflective coating.
- Do not clean the infrared lens too vigorously. This can damage the anti-reflective coating.
- In furnace and other high-temperature applications, you must mount a heatshield on the camera. Using the camera in furnace and other high-temperature applications without a heatshield can cause damage to the camera.
- (Applies only to cameras with an automatic shutter that can be disabled.) Do not disable the automatic shutter in the camera for a prolonged time period (typically max. 30 minutes). Disabling the shutter for a longer time period may harm, or irreparably damage, the detector.
- The encapsulation rating is valid only when all openings on the camera are sealed with their designated covers, hatches, or caps. This includes, but is not limited to, compartments for data storage, batteries, and connectors.
- (Applies only to FLIR A3xx f/A3xx pt series cameras.)
  - Except as described in this manual, do not open the FLIR A3xx pt/A3xx f series camera for any reason. Disassembly of the camera (including removal of the cover) can cause permanent damage and will void the warranty.
  - Do not to leave fingerprints on the FLIR A3xx pt/A3xx f series camera's infrared optics.
  - The FLIR A3xx pt/A3xx f series camera requires a power supply of 24 VDC. Operating the camera outside of the specified input voltage range or the specified operating temperature range can cause permanent damage.
  - When lifting the FLIR A3xx pt series camera use the camera body and base, not the tubes.
- (Applies only to FLIR GF309 cameras.) **CAUTION:** The exceptionally wide temperature range of the FLIR GF309 infrared camera is designed for performing highly accurate electrical and mechanical inspections and can also "see through flames" for inspecting gas-fired furnaces, chemical heaters and coal-fired boilers. IN ORDER TO DERIVE ACCURATE TEMPERATURE MEASUREMENTS IN THESE ENVIRONMENTS THE GF309 OPERATOR MUST HAVE A STRONG UNDERSTANDING OF RADIOMETRIC FUNDAMENTALS AS WELL AS THE PRODUCTS AND CONDITIONS OF COMBUSTION THAT IMPACT REMOTE TEMPERATURE MEASUREMENT. The Infrared Training Center (itc) offers a wide range of world class infrared

actoolsupply.com

actoolsupply.com

training for thermography professionals including GF309 operators. For more information about obtaining the training and certification you require, contact your FLIR sales representative or itc at www.infraredtraining.com.

actoolsupply.com

actoolsupply.com

2 Notice to user

Typographical conventions

This manual uses the following typographical conventions:

- **Semibold** is used for menu names, menu commands and labels, and buttons in dialog boxes.
- *Italic* is used for important information.
- `Monospace` is used for code samples.
- UPPER CASE is used for names on keys and buttons.

User-to-user forums

Exchange ideas, problems, and infrared solutions with fellow thermographers around the world in our user-to-user forums. To go to the forums, visit:

http://www.infraredtraining.com/community/boards/

Calibration

(This notice only applies to cameras with measurement capabilities.)

We recommend that you send in the camera for calibration once a year. Contact your local sales office for instructions on where to send the camera.

Accuracy

(This notice only applies to cameras with measurement capabilities.)

For very accurate results, we recommend that you wait 5 minutes after you have started the camera before measuring a temperature.

For cameras where the detector is cooled by a mechanical cooler, this time period excludes the time it takes to cool down the detector.

Disposal of electronic waste

10742803;a1

As with most electronic products, this equipment must be disposed of in an environmentally friendly way, and in accordance with existing regulations for electronic waste.

Please contact your FLIR Systems representative for more details.

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

3 Customer help

General

For customer help, visit:

http://support.flir.com

Submitting a question

To submit a question to the customer help team, you must be a registered user. It only takes a few minutes to register online. If you only want to search the knowledgebase for existing questions and answers, you do not need to be a registered user.

When you want to submit a question, make sure that you have the following information to hand:

- The camera model
- The camera serial number
- The communication protocol, or method, between the camera and your PC (for example, HDMI, Ethernet, USB™, or FireWire™)
- Operating system on your PC
- Microsoft® Office version
- Full name, publication number, and revision number of the manual

Downloads

On the customer help site you can also download the following:

- Firmware updates for your infrared camera
- Program updates for your PC software
- User documentation
- Application stories
- Technical publications

actoolsupply.com

actoolsupply.com

4 Documentation updates

General

Our manuals are updated several times per year, and we also issue product-critical notifications of changes on a regular basis.

To access the latest manuals and notifications, go to the Download tab at:

http://support.flir.com

It only takes a few minutes to register online. In the download area you will also find the latest releases of manuals for our other products, as well as manuals for our historical and obsolete products.

actoolsupply.com

actoolsupply.com

5 Important note about this manual

General

FLIR Systems issues generic manuals that cover several cameras within a model line.

This means that this manual may contain descriptions and explanations that do not apply to your particular camera model.

NOTE

FLIR Systems reserves the right to discontinue models, software, parts or accessories, and other items, or to change specifications and/or functionality at any time without prior notice.

actoolsupply.com

actoolsupply.com

6 Quick Start Guide

Procedure

Follow this procedure to get started right away:

1	Charge the battery for four hours.
2	Insert the battery into the camera.
3	Insert an SD Memory Card into the card slot at the bottom of the camera.
4	Push the On/Off button to turn on the camera. Allow 45 seconds for the startup sequence.
5	Aim the camera toward your target of interest.
6	Push the Preview/Save button halfway down to autofocus the camera.
7	Push the Preview/Save button fully down to save an image.
8	Do one of the following: ▪ Remove the SD Memory Card and insert it into a card reader connected to a computer. ▪ Connect a computer to the camera using a USB Mini-B cable.
9	Move the image from the card or camera using a drag-and-drop operation.

actoolsupply.com

AC Tool Supply.com
877-207-1244
aikencolon.com

7 Parts lists

7.1 Contents of the transport case

- Battery (2 ea.)
- Battery charger
- Bluetooth headset*
- Calibration certificate
- Camera lens cap
- Downloads brochure
- FLIR ResearchIR software*
- FLIR Tools software
- Hard transport case
- Infrared camera with lens
- Memory card
- Neckstrap
- Power supply, incl. multi-plugs
- Printed Getting Started Guide
- Printed Important Information Guide
- Service & training brochure
- Sunshield
- USB cable
- User documentation CD-ROM
- Video cable
- Warranty extension card

* The inclusion of this item is dependent on model.

NOTE: FLIR Systems reserves the right to discontinue models, parts or accessories, and other items, or to change specifications at any time without prior notice.

7.2 List of accessories

This section contains a list of accessories that you can purchase for your camera.

- 1123970 Sun shield
- 1124544 Neck strap
- 1124545 Pouch
- 1196398 Battery
- 1196818 Lens cap camera
- 1196895 Hard transport case for FLIR T/B2xx-4xx
- 1196960 IR lens, f = 10 mm, 45° incl. case
- 1196961 IR lens, f = 30 mm, 15° incl. case

actoolsupply.com

actoolsupply.com

- 1910423 USB cable Std A <-> Mini-B
- 1910475 Adapter, SD memory card to USB
- 1910490 Cigarette lighter adapter kit, 12 VDC, 1.2 m/3.9 ft.
- 1910582 Video cable
- 19250-100 IR Window 2 in
- 19251-100 IR Window 3 in.
- 19252-100 IR Window 4 in.
- APP-10000 FLIR Viewer (iPad/iPhone Application)
- APP-10001 FLIR Remote (iPad/iPhone Application)
- DSW-10000 FLIR IR Camera Player
- ITC-ADV-3021 ITC Advanced General Thermography Course - attendance, 1 pers.
- ITC-ADV-3029 ITC Advanced General Thermography Course- group of 10 pers.
- ITC-CER-5101 ITC Level 1 Thermography Course - attendance, 1 pers.
- ITC-CER-5105 ITC Level 1 Thermography Course - additional student to on site class, 1 pers
- ITC-CER-5109 ITC Level 1 Thermography Course – group of 10 pers.
- ITC-CER-5201 ITC Level 2 Thermography Course - attendance, 1 pers.
- ITC-CER-5205 ITC Level 2 Thermography Course - additional student to on site class, 1 pers
- ITC-CER-5209 ITC Level 2 Thermography Course – group of 10 pers.
- ITC-CER-6101 EN473 IT Certification course Category 1, excl. Certification, 1 pers.
- ITC-CER-6109 EN473 IT Certification course Category 1, excl. Certification, group up to 10 pers.
- ITC-CON-1001 ITC conference fee
- ITC-EXP-0511 ITC Getting Started with Thermography - attendance, 1 pers.
- ITC-EXP-0521 ITC Getting Started with Thermography (evening or weekend) - attendance, 1 pers.
- ITC-EXP-1001 ITC Training 1 day - attendance 1 pers.
- ITC-EXP-1009 ITC Training 1 day - group up to 10 pers.
- ITC-EXP-1011 ITC Short course Introduction to thermography -attendance 1 pers. (1 day)
- ITC-EXP-1019 ITC Short course Introduction to thermography - inclusive 10 pers. (1 day)
- ITC-EXP-1021 ITC In-house training - additional attendance 1 pers. (per day)
- ITC-EXP-1029 ITC In-house training - group up to 10 pers. (per day)
- ITC-EXP-2001 ITC Training 2 days - attendance 1 pers.
- ITC-EXP-2009 ITC Training 2 days - group up to 10 pers.
- ITC-EXP-2041 ITC Short course electrical thermography - attendance 1 pers. (2 days)
- ITC-EXP-2049 ITC Short course electrical thermography - inclusive 10 pers. (2 days)
- ITC-EXP-3001 ITC Training 3 days - attendance 1 pers.

actoolsupply.com

actoolsupply.com

- ITC-EXP-3009 ITC Training 3 days - group up to 10 pers.
- ITC-FEE-0120 Certification EN473 IT Category 1
- ITC-FEE-0130 Repeat Certification EN473 IT Category 1
- ITC-PRA-2011 ITC Practical Course - Solar panel inspection - attendance, 1 pers (2 days)
- ITC-PRA-2019 ITC Practical Course - Solar panel inspection - group up to 10 pers (2 days)
- ITC-SOW-0001 ITC Software course - attendance 1 pers. (per day)
- ITC-SOW-0009 ITC Software course - group up to 10 pers. (per day)
- ITC-SOW-1001 ITC Training FLIR Software - attendance 1 pers. (1 day)
- ITC-SOW-2001 ITC Training FLIR Software - attendance 1 pers. (2 days)
- ITC-TFT-0100 ITC travel time for instructor
- ITC-TOL-1001 Travel and lodging expenses instructor (Europe, Balcans, Turkey, Cyprus)
- ITC-TOL-1002 Travel and lodging expenses instructor (Russia/GUS, Middle East, North Africa)
- ITC-TOL-1003 Travel and lodging expenses instructor (Center and South Africa)
- ITC-TOL-1004 Travel and lodging expenses instructor (various)
- ITC-TOL-1005 Travel and lodging expenses instructor (other)
- T127451 FLIR Reporter Professional (license only)
- T197000 High temp. option +1200°C/+2192°F for FLIR T/B2xx to T/B4xx and A/SC3xx Series
- T197214 Close-up 2× (50 μm) incl. case
- T197215 Close-up 4× (100 μm) incl. case
- T197408 IR lens, 76 mm (6°) with case and mounting support for T/B-200/400
- T197412 IR lens, 4 mm (90°) with case and mounting support for T/B2xx-4xx
- T197650 2-bay battery charger, incl. power supply with multi plugs
- T197667 Battery package
- T197717 FLIR Reporter Professional (DVD)
- T197771 Bluetooth Headset
- T197965 FLIR Tools
- T198206 FLIR ResearchIR 3.1
- T198206L10 FLIR ResearchIR 3.1, 10 user licenses
- T198206L5 FLIR ResearchIR 3.1, 5 user licenses
- T198209 FLIR ResearchIR Max 3.1
- T198209L10 FLIR ResearchIR Max 3.1, 10 user licenses
- T198209L5 FLIR ResearchIR Max 3.1, 5 user licenses
- T198290 Upgrade FLIR ResearchIR 3.x to FLIR ResearchIR Max 3.1
- T198291 Upgrade previous version to FLIR ResearchIR Max 3.1
- T198292 Upgrade previous version to FLIR ResearchIR 3.1
- T199802 General Maintenance T2xx-4xx series
- T199815 One year extended warranty for T2xx-4xx series

actoolsupply.com

actoolsupply.com

- T910737 Memory card micro-SD with adapters
- T910750 Power supply, incl. multi plugs
- T910972 EX845: Clamp meter + IR therm TRMS 1000A AC/DC
- T910973 MO297: Moisture meter, pinless with memory

NOTE: FLIR Systems reserves the right to discontinue models, parts or accessories, and other items, or to change specifications at any time without prior notice.

actoolsupply.com

AC Tool Supply.com
877-207-1244
aikencolon.com

8 A note about ergonomics

General

To prevent strain injuries, it is important that you hold the camera ergonomically correct. This section gives advice and examples on how to hold the camera.

NOTE

Please note the following:

- Always adjust the angle of the lens to suit your work position.
- When you hold the camera, make sure that you support the camera housing with your left hand too. This decreases the strain on your right hand.

Figure

10758503;a2

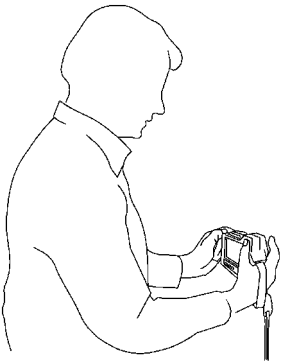

10758603;a2

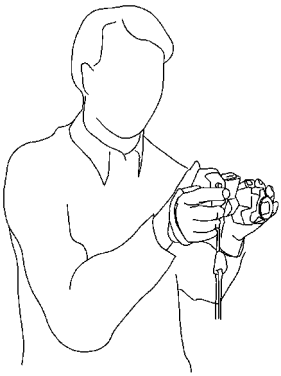

10758803;a2

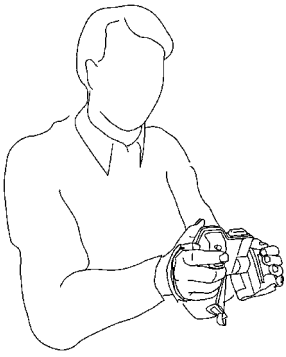

10758703;a2

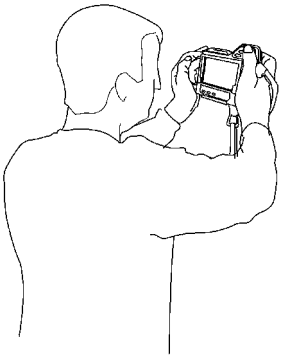

actoolsupply.com

9 Camera parts

9.1 Rear view

Figure

10758903;a2

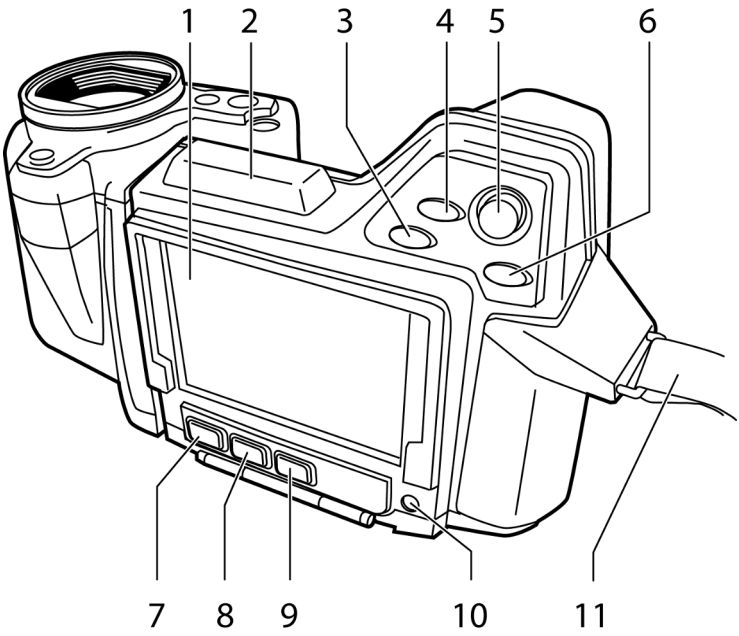

Explanation

This table explains the figure above:

1	Touch screen LCD.
2	Antenna for wireless communication.
3	Digital zoom button.
4	Programmable button.
5	Joystick: Move up/down or left/right to navigate on menus, in dialog boxes, and in the image archive. Push to confirm choices.
6	Menu/Back button: Push to display the menu on the screen, and to go back in dialog boxes.

actoolsupply.com

7	Mode button: Push to display the mode selector and select a camera mode. The modes that can be selected are: ■ **Thermal camera**: Using this mode, the camera captures infrared images. ■ **Digital camera**: Using this mode, the camera captures visual images. ■ **Thermal fusion**: Using this mode, the camera captures an image where some parts are displayed as an infrared image and some parts as a visual image, depending on the temperature. ■ **Picture-in-Picture**: Using this mode, the camera captures an image where the middle part is displayed as an infrared image and the outer frame as a visual image. ■ **MSX** (Multi Spectral Dynamic Imaging): Using this mode, the camera captures infrared images where the edges of the objects are enhanced.
8	A/M button: This button has two main functions: **1** Push to switch between automatic and manual adjustment modes. The manual adjustment modes that can be selected are the following: ■ **Manual**: Using this mode, the top and bottom temperature levels in the scale can be changed simultaneously, by pushing the joystick up/down. The temperature span can be changed by pushing the joystick left/right. ■ **Manual min**: Using this mode, the bottom temperature level in the scale can be changed by pushing the joystick up/down, while the top temperature level remains fixed. ■ **Manual max**: Using this mode, the top temperature level in the scale can be changed by pushing the joystick up/down, while the bottom temperature level remains fixed. **2** Push and hold the button until you hear a clicking sound to autoadjust the image.
9	Archive button: Push to open/close the image gallery.
10	On/Off button: Push to turn on/turn off the camera. Allow 45 seconds for the startup sequence.
11	Hand strap.

actoolsupply.com

actoolsupply.com

9.2 Front view

Figure

10759003;a2

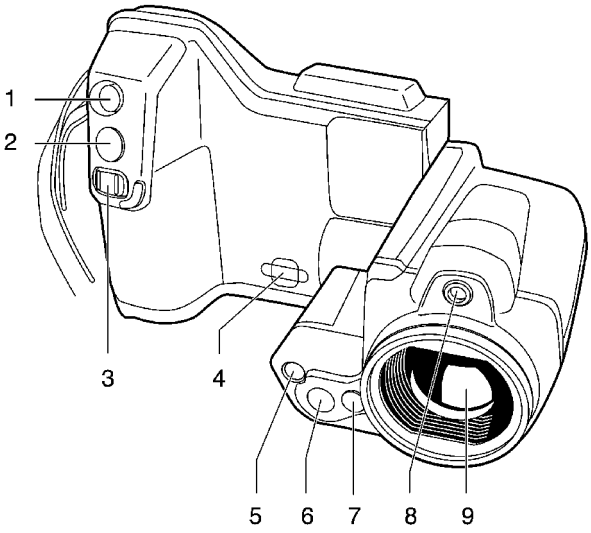

Explanation

This table explains the figure above:

1	Laser pointer button: Push to activate the laser pointer.
2	This button has two main functions: **1** Preview/Save: Push the button fully down to save an infrared image and a digital photo simultaneously. **Note**: The behavior of this button can be changed under **Settings** to one of the following: ■ **Preview**/**Save**. ■ **Save directly** (default). ■ **Always preview**. **2** Autofocus: Push the button halfway down to autofocus the camera.
3	Focus button: Move left/right to manually focus the camera.
4	Attachment point for the neck strap.
5	Video lamp.
6	Digital camera lens.
7	Release button for additional infrared lenses.
8	Laser pointer.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

9	Infrared lens.

NOTE

The laser pointer may not be enabled in all markets.

actoolsupply.com

actoolsupply.com

9.3 Bottom view

Figure

10759103;a2

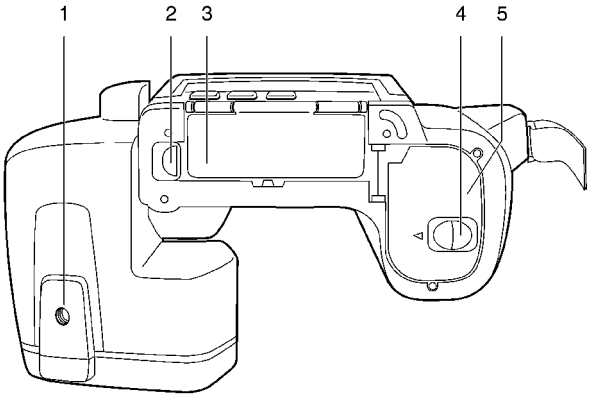

Explanation

This table explains the figure above:

1	Tripod mount 1/4"-20
2	Release button for the cover to the connector bay
3	Cover for the connector bay
4	Release button for the battery compartment cover
5	Cover for the battery compartment

actoolsupply.com

actoolsupply.com

9.4 Battery condition indicator

General

The battery has a battery condition indicator.

Figure

10715703;a3

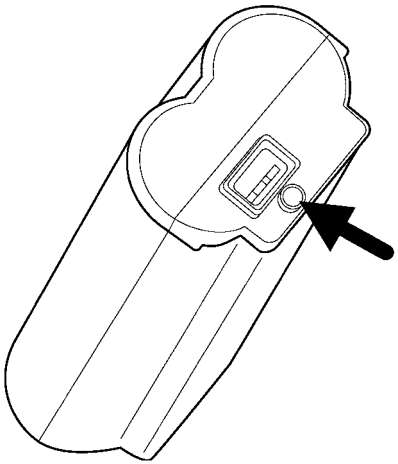

Explanation

This table explains the battery condition indicator:

Type of signal	Explanation
The green light flashes.	The power supply or the stand-alone battery charger is charging the battery.
The green light is continuous.	The battery is fully charged.
The green light is off.	The camera is using the battery (instead of the power supply).

actoolsupply.com

actoolsupply.com

9.5 Laser pointer

General

The camera has a laser pointer. When the laser pointer is on, you can see a laser dot approximately 40 mm (1.57 in.) above the target.

Figure

This figure shows the difference in position between the laser pointer and the optical center of the infrared lens:

10759203;a2

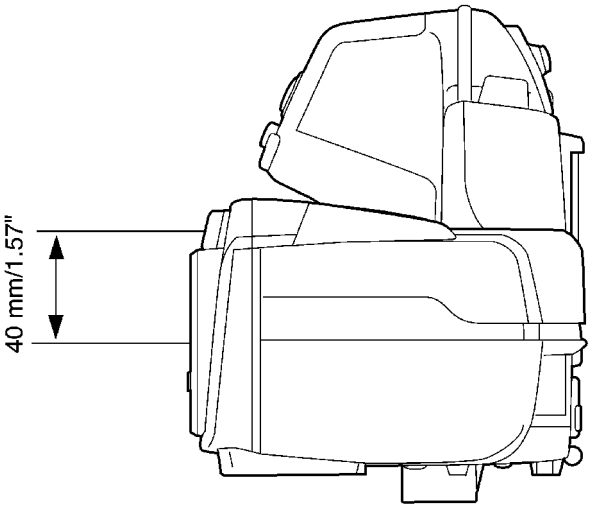

WARNING

Do not look directly into the laser beam. The laser beam can cause eye irritation.

CAUTION

Protect the laser pointer with the protective cap when you are not using the laser pointer.

NOTE

- A laser warning symbol is displayed on the screen when the laser pointer is on.
- The laser pointer may not be enabled in all markets.

Laser warning label

A laser warning label with the following information is attached to the camera:

10743603;a2

LASER RADIATION
DO NOT STARE INTO BEAM
CLASS 2 LASER PRODUCT
WAVELENGTH: 635 nm MAX. OUTPUT POWER: 1 mW
THIS PRODUCT COMPLIES WITH 21 CFR 1040.10 AND 1040.11 EXCEPT FOR DEVIATIONS PURSUANT TO LASER NOTICE NO. 50 DATED JUNE 24, 2007.

Laser rules and regulations

Wavelength: 635 nm. Max. output power: 1 mW.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

This product complies with 21 CFR 1040.10 and 1040.11 except for deviations pursuant to Laser Notice No. 50, dated June 24, 2007.

actoolsupply.com

10 Screen elements

Figure

10760703;a2

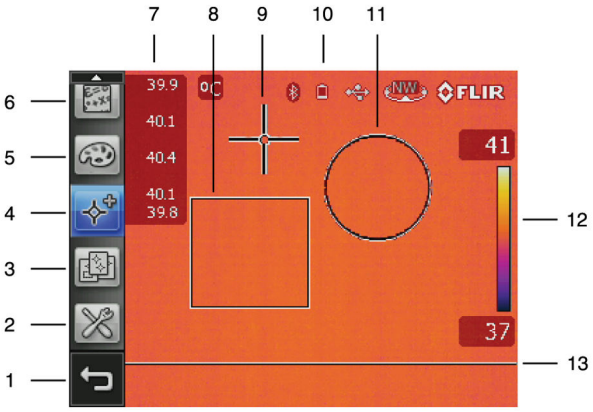

Explanation

This table explains the figure above:

1	Back toolbar button.
2	Mode toolbar button.
3	Presets toolbar button.
4	Tools toolbar button.
5	Palette toolbar button.
6	Parameters toolbar button.
7	Result table.
8	Measurement box.
9	Measurement spotmeter.
10	Various status and mode icons, e.g., Bluetooth, battery, USB, and compass.
11	Measurement circle.
12	Temperature scale.
13	Measurement line.

actoolsupply.com

11 Navigating the menu system

Figure

10763703;a2

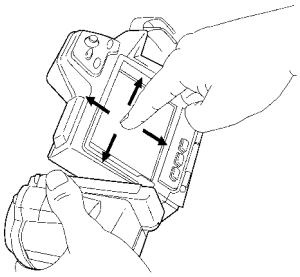

10763603;a2



Explanation

The figure above shows the two ways to navigate the menu system in the camera:

- Using the index finger or a stylus pen to navigate the menu system (left).
- Using the joystick to navigate the menu system (right).

You can also use a combination of the two.

In this manual it is assumed that the joystick is used, but most tasks can also be carried out using the index finger or a stylus pen.

actoolsupply.com

actoolsupply.com

12 External devices and storage media

Figure

10759303;a4

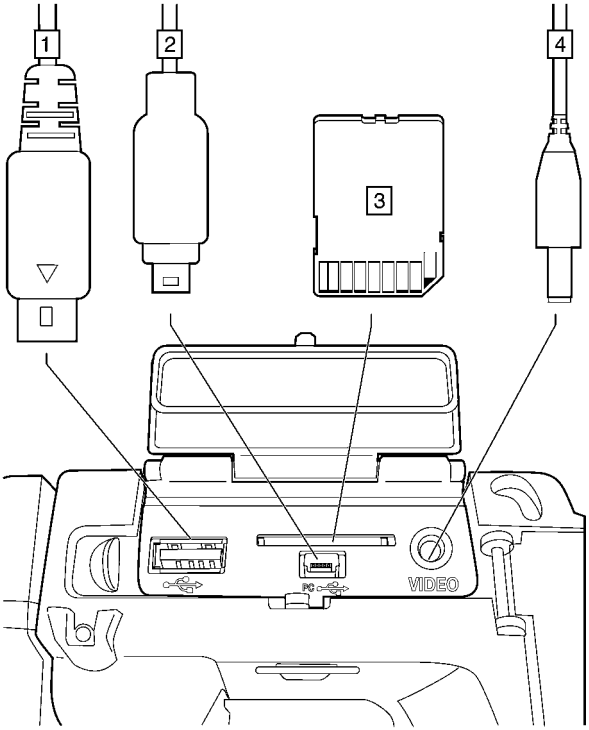

Explanation

This table explains the figure above:

1	To connect an external USB device to the camera, use a USB-A cable and this socket.
2	To connect a computer to the camera to move images and files to and from the camera, use a USB Mini-B cable and this socket.
3	To insert an SD memory card, use this card slot.
4	To connect a video monitor to the camera, use a CVBS (composite video) cable and this socket.

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

13 Pairing Bluetooth devices

General

Before you can use a Bluetooth device with the camera, you need to pair the devices.

Procedure

Follow this procedure:

1	Turn on the camera.
2	Push the Menu/Back button.
3	On the main menu, go to the **Mode** button and push the joystick.
4	On the **Mode** menu, select **Settings** and push the joystick.
5	On the **Connectivity** tab, go to **Bluetooth** and push the joystick to enable Bluetooth connectivity.
6	On the same tab, go to **Add Bluetooth device** and push the joystick to begin scanning for devices. At this stage you need to refer to the user documentation for your Bluetooth device.

actoolsupply.com

14 Fetching data from external Extech meters

General

You can fetch data from an external Extech meter and merge this data into the result table in the infrared image.

Figure

T638370;a1

Supported Extech meters

- Extech Moisture Meter MO297
- Extech Clamp Meter EX845

Technical support for Extech meters

This support is for Extech meters only. For technical support for infrared cameras.

NOTE

- This procedure assumes that you have paired the Bluetooth devices and set the functionality of the Save button to Preview/Save.

Procedure

Follow this procedure:

1	Turn on the camera.
2	Turn on the Extech meter.

actoolsupply.com

actoolsupply.com

3	On the meter, enable Bluetooth mode. Refer to the user documentation for the meter for information on how to do this.
4	On the meter, choose the quantity that you want to use (voltage, current, resistance, etc.). Refer to the user documentation for the meter for information on how to do this. Results from the meter will now automatically be displayed in the result table in the top left corner of the infrared camera screen.
5	Do one of the following: ▪ To preview an image, push the Preview/Save button. At this stage, you can add additional values. To do so, take a new measurement with the meter and select **Add** on the infrared camera screen. ▪ To save an image without previewing, push and hold down the Preview/Save button. ▪ (Dependent on camera model) To add a value to a recalled image, turn on the meter after you have recalled the image, then select **Add** on the infrared camera screen. A maximum of eight values can be added, but note that some values are broken into two lines.

actoolsupply.com

actoolsupply.com

14.1 Typical moisture measurement and documentation procedure

General

The following procedure can form the basis for other procedures using Extech meters and infrared cameras.

Procedure

Follow this procedure:

1	Use the infrared camera to identify any potential damp areas behind walls and ceilings.
2	Use the moisture meter to measure the moisture levels at various suspect locations that may have been found.
3	When a spot of particular interest is located, store the moisture reading in the moisture meter's memory and identify the measurement spot with a handprint or other thermal identifying marker.
4	Recall the reading from the meter memory. The moisture meter will now continuously transmit this reading to the infrared camera.
5	Use the camera to take a thermal image of the area with the identifying marker. The stored data from the moisture meter will also be saved on the image.

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

15 Handling the camera

15.1 Charging the battery

NOTE

You must charge the battery for four hours before you start using the camera for the first time.

General

You must charge the battery when a low battery voltage warning is displayed on the screen.

Follow one of these procedures to charge the battery:

- Use the combined power supply and battery charger to charge the battery when it is inside the camera.
- Use the combined power supply and battery charger to charge the battery when it is outside the camera.
- Use the stand-alone battery charger to charge the battery

actoolsupply.com

actoolsupply.com

15.1.1 Using the combined power supply and battery charger to charge the battery when it is inside the camera

NOTE

For brevity, the ‘combined power supply and battery charger’ is called the ‘power supply’ below.

Procedure

Follow this procedure to use the power supply to charge the battery when it is inside the camera:

1	Open the battery compartment lid.
2	Connect the power supply cable plug to the connector on the battery.
3	Connect the power supply mains-electricity plug to a mains socket.
4	Disconnect the power supply cable plug when the green light of the battery condition indicator is continuous.

SEE ALSO

For information about the battery condition indicator, see section 9.4 – Battery condition indicator on page 20.

actoolsupply.com

actoolsupply.com

15.1.2 Using the combined power supply and battery charger to charge the battery when it is outside the camera

NOTE

For brevity, the ‘combined power supply and battery charger’ is called the ‘power supply’ below.

Procedure

Follow this procedure to use the power supply to charge the battery when it is outside the camera:

1	Put the battery on a flat surface.
2	Connect the power supply cable plug to the connector on the battery.
3	Connect the power supply mains-electricity plug to a mains socket.
4	Disconnect the power supply cable plug when the green light of the battery condition indicator is continuous.

SEE ALSO

For information about the battery condition indicator, see section 9.4 – Battery condition indicator on page 20.

actoolsupply.com

actoolsupply.com

15.1.3 Using the stand-alone battery charger to charge the battery

Procedure

Follow this procedure to use the stand-alone battery charger to charge the battery:

1	Put the battery in the stand-alone battery charger.
2	Connect the power supply cable plug to the connector on the stand-alone battery charger.
3	Connect the power supply mains-electricity plug to a mains socket.
4	Disconnect the power supply cable plug when the green light of the battery condition indicator is continuous.

SEE ALSO

For information about the battery condition indicator, see section 9.4 – Battery condition indicator on page 20.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

15.2 Inserting the battery

NOTE

Use a clean, dry cloth to remove any water or moisture on the battery before you insert it.

Procedure

Follow this procedure to insert the battery:

1	Push the release button on the battery compartment cover to unlock it. 10759603;a1 
2	Open the cover to the battery compartment. 10759703;a1 
3	Push the battery into the battery compartment until the battery locking mechanism engages. 10759803;a1 

actoolsupply.com

actoolsupply.com

4	Close the cover to the battery compartment. 10759903;a1 

actoolsupply.com

actoolsupply.com

15.3 Removing the battery

Procedure

Follow this procedure to remove the battery:

1	Push the release button on the battery compartment cover to unlock it. 10759603;a1 
2	Open the cover to the battery compartment. 10763903;a1 
3	Push the red release button in the direction of the arrow to unlock the battery. 10760003;a2 

actoolsupply.com

actoolsupply.com

4	Pull out the battery from the battery compartment. 10760103;a1 

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

15.4 Turning on and turning off the camera

- To turn on the camera, push and release the On/Off button.
- To turn off the camera, push and release the On/Off button.

actoolsupply.com

actoolsupply.com

15.5 Adjusting the angle of lens

General

To make your working position as comfortable as possible, you can adjust the angle of the lens.

Figure

10760203;a2

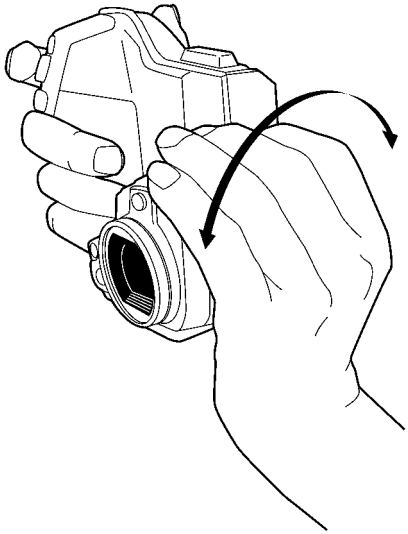

Procedure

To adjust the angle, tilt the lens up or down.

actoolsupply.com

actoolsupply.com

15.6 Attaching the sunshield

General

You can attach a sunshield to the camera to make the LCD screen easier to see in sunlight.

Procedure

Follow this procedure to attach the sunshield to the camera:

1	Align the two front tabs of the sunshield with the corresponding two notches at the top of the screen. 10765203;a2 
2	Push the front part of the sunshield into position. Make sure that the two tabs mate with the corresponding notches. 10765303;a2 
3	Carefully hold together the two rear wings of the sunshield. 10765403;a2 

actoolsupply.com

actoolsupply.com

4	Push the rear part of the sunshield toward the screen, and then release your grip. Make sure that the two tabs mate with the corresponding notches. 10765503;a2 

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

15.7 Using the laser pointer

Figure

10760303;a2

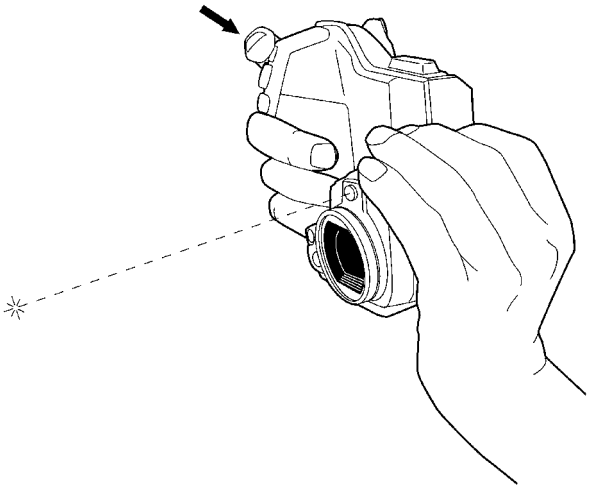

Procedure

Follow this procedure to use the laser pointer:

1	To turn on the laser pointer, push and hold the laser pointer button.
2	To turn off the laser pointer, release the laser pointer button.

NOTE

The laser pointer may not be enabled in all markets.

actoolsupply.com

actoolsupply.com

16 Working with images and folders

16.1 Adjusting the infrared camera focus

Procedure

To adjust the infrared camera focus, do one of the following:

- Push the focus button left for far focus.
- Push the focus button right for near focus.
- Push the Preview/Save button halfway down to autofocus the camera.

NOTE

It is important that you hold the camera steady while autofocusing.

actoolsupply.com

actoolsupply.com

16.2 Previewing an image

General

In preview mode, you can add various types of annotations to the image before you save it, such as a text, a table with textual information, a voice comment, a sketch, etc. You do this by selecting the type of annotation on the toolbar that is automatically displayed when you preview an image.

In preview mode you can also check that the image contains the required information before you save it to the SD Memory Card.

Procedure

Follow this procedure:

1	When the camera leaves the factory, it is configured to save an image directly, without previewing. To enable previewing, do the following: **1** Push the Menu/Back button. **2** On the main menu, go to the **Mode** button and push the joystick. **3** On the **Mode** menu, select **Settings** and push the joystick. **4** On the **Preferences** tab, go to **Save button** and select **Always preview**.
2	To preview an image, push the Preview/Save button fully down.

actoolsupply.com

actoolsupply.com

16.3 Saving an image

General

You can save one or more images to the SD Memory Card.

Formatting memory cards

For best performance, memory cards should be formatted to the FAT (FAT16) file system. Using FAT32-formatted memory cards may result in inferior performance. To format a memory card to FAT (FAT16), follow this procedure:

1	Insert the memory card into a card reader that is connected to your computer.
2	In Windows Explorer, select **My Computer** and right-click the memory card.
3	Select **Format**.
4	Under **File system**, select **FAT**.
5	Click **Start**.

Image capacity

This table gives information on the *approximate* number of images that can be saved on SD Memory Cards:

Card size	No voice annotation	Incl. 30 seconds voice annotation
256 MB	500	250
512 MB	1000	500
1 GB	2000	1000

Procedure

To save an image without previewing, push the Preview/Save button fully down.

NOTE

The behavior of the Preview/Save button can be changed on the **Preferences** tab (**Mode** > **Settings** > **Preferences**).

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

16.4 Periodically saving an image

General

You can periodically save images to the SD Memory card.

Procedure

Follow this procedure to periodically save an image:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Program** and push the joystick.

4	Use the joystick to set the desired parameters. These include the following:
	▪ Duration between images.
	▪ Stop conditions:
	  ▪ **Manually**.
	  ▪ **Number of images**.
	  ▪ **Total time duration**.

5	Push the Menu/Back button.
6	▪ To start the periodic saving, push the Preview/Save button fully down. ▪ To stop the periodic saving, push the Preview/Save button fully down.

actoolsupply.com

actoolsupply.com

16.5 Opening an image

General

When you save an image, it is stored on the SD Memory Card. To display the image again, you can recall it from the SD Memory Card.

Procedure

Follow this procedure:

1	Push the Archive button to display a thumbnail view of recently saved images.
2	Move the joystick left/right or up/down to select a specific image.
3	Push the joystick to display the image.

NOTE

To leave archive mode, push the Archive button.

actoolsupply.com

actoolsupply.com

16.6 Adjusting an image manually

General

An image can be adjusted *automatically* or *manually*.

You use the A/M button to switch between these two modes

Example 1

This figure shows two infrared images of cable connection points. In the left image a correct analysis of the circled cable is difficult if you only auto-adjust the image. You can analyze this cable in more detail if you

- change the temperature scale level
- change the temperature scale span.

In the left image, the image is auto-adjusted. In the right image the maximum and minimum temperature levels have been changed to temperature levels near the object. On the temperature scale to the right of each image you can see how the temperature levels were changed.

10577503;a2

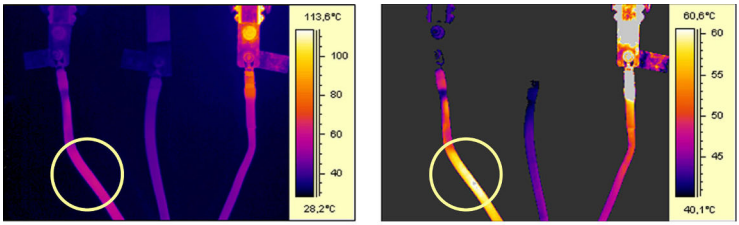

A (automatic) M (manual)

actoolsupply.com

actoolsupply.com

Example 2

This figure shows two infrared images of an isolator in a power line.

In the left image, the cold sky and the power line structure are recorded at a minimum temperature of –26.0°C (–14.8°F). In the right image the maximum and minimum temperature levels have been changed to temperature levels near the isolator. This makes it easier to analyze the temperature variations in the isolator.

10742503;a3

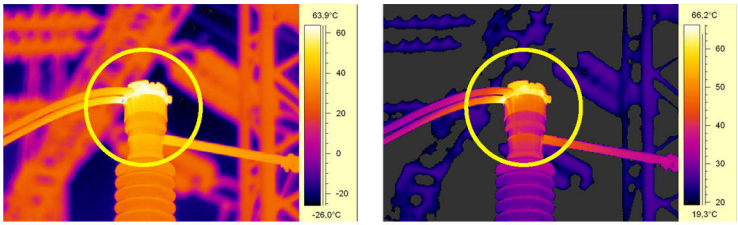

A (automatic) M (manual)

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

Changing the temperature scale level

Follow this procedure to change the temperature scale level:

1	Push the A/M button repeatedly to select one of the following manual modes: ▪ **Manual** ▪ **Manual max.** ▪ **Manual min.**
2	To change the temperature scale level (-s), move the joystick up/down.

Changing the temperature scale span

Follow this procedure to change the temperature scale span:

1	Push the A/M button repeatedly to select **Manual** .
2	To change the temperature span, move the joystick left/right.

actoolsupply.com

actoolsupply.com

16.7 Hiding overlay graphics

General

Overlay graphics provide information about an image. You can choose to hide some or all overlay graphics.

Procedure

Follow this procedure:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Preferences** tab, go to **View** and disable the overlay graphics that you do not want to display.

actoolsupply.com

actoolsupply.com

16.8 Deleting images

General

You can delete one or more images from the SD Memory Card.

Procedure

Follow this procedure to delete an image:

1	Push the Archive button.
2	Select the image you want to delete by using the joystick.
3	Push the joystick to open the image.
4	Push the joystick to display a menu.
5	On the menu, select one of the following: ■ **Delete**. ■ **Delete all**.
6	Push the joystick to confirm.

actoolsupply.com

actoolsupply.com

16.9 Creating an Adobe PDF report

General

You can create an Adobe PDF report about any image on the SD Memory Card. The report may include the following:

- The infrared image, including any associated visual image.
- A list of text annotations.
- A list of measurement results.
- A list of object parameters.
- A sketch.
- An image description.

Procedure

Follow this procedure:

1	Insert a USB memory stick into the USB connector.
2	Push the Archive button.
3	Select the image for which you want to create a report.
4	Push the joystick to open the image.
5	Push the joystick to display a menu.
6	On the menu, select **Create report page** by using the joystick. At this stage you can also add information to the report header and footer.

NOTE

To view the report on the PC, you need Adobe Reader. This software can be downloaded for free from:

http://get.adobe.com/reader/

actoolsupply.com

AC Tool Supply.com
877-207-1244
aikencolon.com

17 Working with fusion

What is fusion?

Fusion is a function that lets you display part of a digital photo as an infrared image.

For example, you can set the camera to display all areas of an image that have a certain temperature in infrared, with all other areas displayed as a digital photo. You can also set the camera to display an infrared image frame on top of a digital photo. You can then move around the infrared image frame, or change the size of the image frame.

Fusion types

Depending on camera model, up to four different types of fusion are available. These are:

- **Above**: All areas in the digital photo with a temperature above the specified temperature level are displayed in infrared.
- **Below**: All areas in the digital photo with a temperature below the specified temperature level are displayed in infrared.
- **Interval**: All areas in the digital photo with a temperature between two specified temperature levels are displayed in infrared.
- **Picture in Picture**: An infrared image frame is displayed on top of the digital photo.

actoolsupply.com

actoolsupply.com

Image examples

This table explains the four different types of fusion:

Fusion type	Image
Above	
Below	
Interval	
Picture in Picture	

actoolsupply.com

actoolsupply.com

Procedure

Follow this procedure to set up a fusion type:

1	Push the Mode button to select one of the following: ■ **Thermal fusion** . ■ **Picture-in-Picture** .
2	Push the A/M button to select one of the following: ■ **Above**. ■ **Below** ■ **Interval**
3	(This step applies to **Thermal fusion**.) Do one or more of the following: ■ If you chose **Above** or **Below**, move the joystick up or down to adjust the temperature level. The temperature level that you set will be the level beyond which the infrared image will be displayed as a visual photo. ■ If you chose **Interval**, do one or more of the following: ■ Push the joystick up/down to move the interval up/down. ■ Push the joystick left/right to increase/decrease the interval. The temperature levels that you set will be the level beyond which the infrared image will be displayed as a visual photo.
4	(This step applies to **Picture-in-Picture**.) Do one or more of the following: ■ If you chose **Above** or **Below**, move the joystick up or down to adjust the temperature level in the infrared portion of the image. ■ If you chose **Interval**, do one or more of the following: ■ Push the joystick up/down to move the temperature interval up/down in the infrared portion of the image. ■ Push the joystick left/right to increase/decrease the temperature interval in the infrared portion of the image.
5	To deactivate **Fusion**, push the Mode button to select **Thermal camera**.

actoolsupply.com

actoolsupply.com

18 Recording video clips

General

You can record non-radiometric infrared or visual video clips. In this mode, the camera can be regarded as an ordinary digital video camera.

The video clips can be played back in Windows Media Player, but it will not be possible to retrieve radiometric information from the video clips.

Procedure

Follow this procedure to record a video clip:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Video** and push the joystick. This will display a notification indicating that the recording has started.
4	To stop the video recording, push the joystick again. When you stop the video recording you can play back the recording in the camera, using the tools on the video recording toolbar.

NOTE

- You can only view the most recently recorded video clips in this mode. To view another video clip, go to the archive mode.
- You can play back the video clips in, for example, Windows Media Player. However, to do so you must also buy, download, and install the 3ivx D4 Decoder, which is an MPEG-4 toolkit that supports MPEG-4 Video, MPEG-4 Audio, and the MP4 file format. You can download the 3ivx D4 Decoder from http://www.3ivx.com/.
- Other video players may also work, for example ffdshow from http://sourceforge.net/projects/ffdshow.
- Codecs may also be available from http://www.free-codecs.com/.
- FLIR Systems does not take any responsibility for the functionality of third-party video players and codecs.

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

19 Working with measurement tools and isotherms

19.1 Setting up measurement tools

General

To measure the temperature, you use one or more measurement tools. This section gives you examples how you set up a spotmeter or an area.

Procedure

Follow this procedure to set up a spotmeter or an area:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select one of the following: ▪ **Add spot** . ▪ **Add box** . ▪ **Add circle** .

NOTE

The area inside the center of the spotmeter must be covered by the object of interest, to display a correct temperature.

For accurate measurements, you must set the object parameters. See section 19.7 – Changing object parameters on page 66.

actoolsupply.com

19.2 Setting up a difference calculation

General

You can let the camera calculate the temperature difference between, for example, a spotmeter and an area. This assumes that you have previously set up at least two measurement tools.

Procedure

Follow this procedure to set up a difference calculation:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Add difference** . This will display a dialog box where you can select the two measurement tools from which you want to calculate the difference.
4	Push the joystick to confirm the choice.

actoolsupply.com

actoolsupply.com

19.3 Setting up isotherms

General

You can make the camera display an isotherm color when certain measurement conditions are met. The following isotherms can be set up:

- An isotherm color that is displayed when a temperature rises above a preset value.
- An isotherm color that is displayed when a temperature falls below a preset value.
- An isotherm color that is displayed when a temperature is between two values.
- An isotherm color that is displayed when the camera detects an area where there may be a risk of humidity in a building structure.
- An isotherm color that is displayed when the camera detects what may be an insulation deficiency in a wall.

Setting up a high-temperature isotherm

Follow this procedure to set up an isotherm color that is displayed when a temperature rises above a preset value:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Add isotherm** and push the joystick.
4	Select **Above**.
5	Move the joystick up/down to set the temperature at which you want the isotherm color to be displayed. The screen will now display the isotherm color when the temperature exceeds the set temperature level.

Setting up a low-temperature isotherm

Follow this procedure to set up an isotherm color that is displayed when a temperature falls below a preset value:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Add isotherm** and push the joystick.
4	Select **Below**.
5	Move the joystick up/down to set the temperature at which you want the isotherm color to be displayed. The screen will now display the isotherm color when the temperature falls below the set temperature level.

Setting up an interval isotherm

Follow this procedure to set up an isotherm color that is displayed when a temperature is between two preset values:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.

actoolsupply.com

actoolsupply.com

3	On the **Tools** menu, select **Add isotherm** and push the joystick.
4	Select **Interval**.
5	Do one of the following: ▪ Move the joystick up/down to set the temperature levels *between which* you want the isotherm color to be displayed. ▪ Move the joystick left/right to set the temperature span *within which* you want the isotherm color to be displayed. The screen will now display the isotherm color when the temperature is between the set temperature levels.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

Setting up a humidity isotherm

Follow this procedure to set up an isotherm color that is displayed when the camera detects an area where there may be a risk of humidity in a building structure:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Add isotherm** and push the joystick.
4	Select **Humidity**.
5	Use the joystick to set the following parameters: ▪ **Rel. humidity limit**: The critical limit of relative humidity that you want to detect in a building structure. For example, mold will grow in areas where the relative humidity is less than 100%, and you may want to find such areas. ▪ **Rel. hum.**: The current relative humidity at the inspection site. ▪ **Atm. temp.**: The current atmospheric temperature at the inspection site.

Setting up an insulation isotherm

Follow this procedure to set up an isotherm color that is displayed when the camera detects what may be an insulation deficiency in a wall:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Add isotherm** and push the joystick.
4	Select **Insulation**.
5	Use the joystick to set the following parameters: ▪ **Inside temp.**: The temperature inside the building you are inspecting. ▪ **Outside temp.**: The temperature outside the building you are inspecting. ▪ **Thermal index**: The accepted energy loss through the wall. Different building codes recommend different values, but typical values are 60–80 for new buildings. Refer to your national building code for recommendations.

actoolsupply.com

actoolsupply.com

19.4 Removing measurement tools

Procedure

Follow this procedure to remove a spotmeter or an area:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Adjust tools** and push the joystick.
4	Select the measurement tool that you wish to remove. This will display a submenu.
5	On the submenu, select **Remove** and push the joystick.

actoolsupply.com

actoolsupply.com

19.5 Moving measurement tools

Procedure

Follow this procedure to move a measurement tool:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Adjust tools** and push the joystick.
4	Select the measurement tool that you wish to move. This will display a submenu.
5	On the submenu, select **Move** and push the joystick. This will make the center of the measurement tool turn blue. You can now move the measurement tool using the joystick.

actoolsupply.com

actoolsupply.com

19.6 Resizing areas

Procedure

Follow this procedure to resize an area:

1	Push the Menu/Back button.
2	On the main menu, go to the **Tools** button and push the joystick.
3	On the **Tools** menu, select **Adjust tools** and push the joystick.
4	Select the measurement tool that you wish to move. This will display a submenu.
5	On the submenu, select **Resize** and push the joystick. This will create resizing handles for the area. You can now resize the area using the joystick.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

19.7 Changing object parameters

General

For accurate measurements, you must set the object parameters. This procedure describes how to change the parameters.

Types of parameters

The camera can use these object parameters:

- **Emissivity**, which determines how much of the radiation originates from the object as opposed to being reflected by it.
- **Reflected apparent temperature**, which is used when compensating for the radiation from the surroundings reflected by the object into the camera. This property of the object is called reflectivity.
- **Object distance**, i.e. the distance between the camera and the object of interest.
- **Atmospheric temperature**, i.e. the temperature of the air between the camera and the object of interest.
- **Relative humidity**, i.e. the relative humidity of the air between the camera and the object of interest.
- **External optics temperature**, i.e., the temperature of any protective windows etc. that are set up between the camera and the object of interest. If no protective window or protective shield is used, this value is irrelevant.
- **External optics transmission**, i.e., the optical transmission of any protective windows, etc. that are set up between the camera and the object of interest.

Recommended values

If you are unsure about the values, the following are recommended:

Atmospheric temperature	+20°C (+69°F)
Emissivity	0.95
Object distance	1.0 m (3.3 ft.)
Reflected apparent temperature	+20°C (+69°F)
Relative humidity	50%

actoolsupply.com

actoolsupply.com

Procedure

Follow this procedure to change the object parameters globally:

1	Push the Menu/Back button.
2	On the main menu, go to the **Parameters** button and push the joystick.
3	On the **Parameters** menu, select the parameter that you want to change and push the joystick.
4	Move the joystick up/down to change the value.
5	Push the joystick to confirm.

NOTE

Of the five parameters above, *emissivity* and *reflected apparent temperature* are the two most important to set correctly in the camera.

SEE ALSO

For more information about parameters, and how to correctly set emissivity and reflected apparent temperature, see section 28 – Thermographic measurement techniques on page 101.

actoolsupply.com

actoolsupply.com

20 Annotating images

General

This section describes how to save additional information to an infrared image by using annotations.

The reason for using annotations is to make reporting and post-processing more efficient by providing essential information about the image, such as conditions, photos, sketches, where it was taken, and so on.

actoolsupply.com

actoolsupply.com

20.1 Adding a digital photo automatically

General

When you save an infrared image you can *automatically* add a digital photo of the object of interest. This digital photo will be associated with the infrared image, which will simplify post-processing and reporting in, for example, FLIR Reporter.

Procedure

Follow this procedure:

1	Make sure that the camera is configured to save a digital photo simultaneously: **1** Push the Menu/Back button. **2** On the main menu, go to the **Mode** button and push the joystick. **3** On the **Mode** menu, select **Settings** and push the joystick. **4** On the **Preferences** tab, enable **Simultaneously save photo**.
2	To automatically add a digital photo, push the Preview/Save button fully down.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

20.2 Adding a digital photo manually

General

When you save an infrared image you can *manually* add a digital photo of the object of interest. This digital photo will be associated with the infrared image, which will simplify post-processing and reporting in, for example, FLIR Reporter.

NOTE

This section assumes that the camera is configured to *always preview* an image before saving it to the memory card.

To configure the camera to always preview, follow this procedure:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Preferences** tab, go to **Save button** and select **Always preview**.

Procedure

Follow this procedure:

1	Push the Preview/Save button fully down.
2	On the toolbar at the bottom of the screen, select .
3	On the menu that is displayed, select **Digital camera photo** and push the joystick.
4	Push the Preview/Save button to save the digital photo.

actoolsupply.com

actoolsupply.com

20.3 Adding a voice annotation

General

A voice annotation is an audio recording that is saved in an infrared image.

The voice annotation is recorded using a Bluetooth microphone headset. The recording can be played back in the camera, and in image analysis and reporting software from FLIR Systems.

NOTE

This section assumes that the camera is configured to *always preview* an image before saving it to the memory card.

To configure the camera to always preview, follow this procedure:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Preferences** tab, go to **Save button** and select **Always preview**.

Procedure

Follow this procedure:

1	Make sure that the Bluetooth headset is turned on and paired with the camera.
2	Push the Preview/Save button fully down.
3	On the toolbar at the bottom of the screen, select .
4	On the menu that is displayed, select **Voice** and push the joystick. This will display a voice annotation toolbar.
5	Use the joystick to record, stop, play back the voice annotation.

actoolsupply.com

actoolsupply.com

20.4 Adding a table

General

A table with textual information can be saved in an infrared image.

This feature is a very efficient way of recording information when you are inspecting a large number of similar objects. The idea behind using a table with textual information is to avoid filling out forms or inspection protocols manually.

Definition of label and value

The concept of *table* in this particular context is based on two important definitions – *label* and *value*. The following examples explains the difference between the two definitions.

Label (examples)	Value (examples)
Company	Company A Company B Company C
Building	Workshop 1 Workshop 2 Workshop 3
Section	Room 1 Room 2 Room 3
Equipment	Tool 1 Tool 1 Tool 3
Recommendation	Recommendation 1 Recommendation 2 Recommendation 3

Procedure

Follow this procedure:

1	Push the Preview/Save button fully down.
2	On the toolbar at the bottom of the screen, select .

actoolsupply.com

actoolsupply.com

3	On the menu that is displayed, select **Table** and push the joystick. This will display a tabular form. T639496;a1 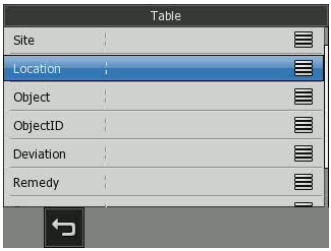
4	Use the joystick to select one of the labels (e.g., Site, Location, Object), then push the joystick. This will display a dialog box where you can create new or edit existing values. T639497;a1 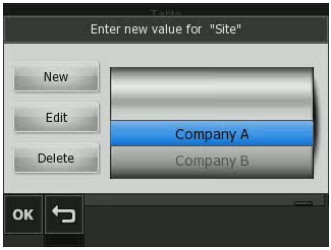
5	Carry out the changes that you want to do, then click **OK** or push the joystick.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

20.5 Adding an text

General

You can add a free-text description that is saved in the infrared image.

NOTE

This section assumes that the camera is configured to *always preview* an image before saving it to the memory card.

To configure the camera to always preview, follow this procedure:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Preferences** tab, go to **Save button** and select **Always preview**.

Procedure

Follow this procedure:

1	Push the Preview/Save button fully down.
2	On the toolbar at the bottom of the screen, select .
3	On the menu that is displayed, select **Text** and push the joystick. This will display a keyboard on the screen.
4	Type the text that you want to add, then click **OK** or push the joystick.

actoolsupply.com

actoolsupply.com

20.6 Adding a sketch

General

A sketch is freehand drawing that you create on a drawing board separate from the infrared image using your index finger or a stylus pen. You can use the sketch feature to create a simple drawing, write down comments, dimensions, etc.

NOTE

This section assumes that the camera is configured to *always preview* an image before saving it to the memory card.

To configure the camera to always preview, follow this procedure:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Preferences** tab, go to **Save button** and select **Always preview**.

Procedure

Follow this procedure:

1	Push the Preview/Save button fully down.
2	On the toolbar at the bottom of the screen, select .
3	On the menu that is displayed, select **Sketch** and push the joystick. This will display drawing board where you can create the sketch.
4	Type the text that you want to add, then click **OK** or push the joystick.

actoolsupply.com

21 Changing settings

21.1 Changing camera settings

General

On this tab you can change the following:

- Temperature range, i.e. the temperature range used for measuring objects. You must change the temperature range according to the expected temperature of the object you are inspecting.
- Add-on lens.
- Display intensity.
- Auto power off.
- Digital camera lamp.
- Calibrate touchscreen.
- Calibrate compass.

Procedure

Follow this procedure to change one or more of the aforementioned settings:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Camera** tab, go to the setting that you want to change.
5	Push the joystick.
6	Move the joystick up/down to select a new value.
7	Push the joystick to confirm.

actoolsupply.com

actoolsupply.com

21.2 Changing preferences

General

On this tab you can change the following:

- Save button.
- Simultaneously save photo.
- Same field of view.
- Programmable button.
- Visibility of overlay graphics.

Procedure

Follow this procedure to change one or more of the aforementioned settings:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Preferences** tab, go to the setting that you want to change.
5	Push the joystick.
6	Move the joystick up/down to select a new value.
7	Push the joystick to confirm.

actoolsupply.com

actoolsupply.com

21.3 Changing connectivity

General

On this tab you can change the following:

- Wi-Fi.
- Bluetooth.

Procedure

Follow this procedure to change one or more of the aforementioned settings:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Connectivity** tab, go to the setting that you want to change.
5	Push the joystick.
6	Move the joystick up/down to select a new value.
7	Push the joystick to confirm.

actoolsupply.com

actoolsupply.com

21.4 Changing regional settings

General

On this tab you can change the following:

- Language.
- Time zone.
- Set date and time.
- Date format.
- Time format.
- Temperature unit.
- Distance unit.

Procedure

Follow this procedure to change one or more of the aforementioned settings:

1	Push the Menu/Back button.
2	On the main menu, go to the **Mode** button and push the joystick.
3	On the **Mode** menu, select **Settings** and push the joystick.
4	On the **Regional** tab, go to the setting that you want to change.
5	Push the joystick.
6	Move the joystick up/down to select a new value.
7	Push the joystick to confirm.

actoolsupply.com

actoolsupply.com

22 Cleaning the camera

22.1 Camera housing, cables, and other items

Liquids

Use one of these liquids:

- Warm water
- A weak detergent solution

Equipment

A soft cloth

Procedure

Follow this procedure:

1	Soak the cloth in the liquid.
2	Twist the cloth to remove excess liquid.
3	Clean the part with the cloth.

CAUTION

Do not apply solvents or similar liquids to the camera, the cables, or other items. This can cause damage.

actoolsupply.com

actoolsupply.com

22.2 Infrared lens

Liquids

Use one of these liquids:

- 96% isopropyl alcohol.
- A commercial lens cleaning liquid with more than 30% isopropyl alcohol.

Equipment

Cotton wool

Procedure

Follow this procedure:

1	Soak the cotton wool in the liquid.
2	Twist the cotton wool to remove excess liquid.
3	Clean the lens one time only and discard the cotton wool.

WARNING

Make sure that you read all applicable MSDS (Material Safety Data Sheets) and warning labels on containers before you use a liquid: the liquids can be dangerous.

CAUTION

- Be careful when you clean the infrared lens. The lens has a delicate anti-reflective coating.
- Do not clean the infrared lens too vigorously. This can damage the anti-reflective coating.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

22.3 Infrared detector

General

Even small amounts of dust on the infrared detector can result in major blemishes in the image. To remove any dust from the detector, follow the procedure below.

NOTE

- This section only applies to cameras where removing the lens exposes the infrared detector.
- In some cases the dust cannot be removed by following this procedure: the infrared detector must be cleaned mechanically. This mechanical cleaning must be carried out by an authorized service partner.

CAUTION

In Step 2 below, do not use pressurized air from pneumatic air circuits in a workshop, etc., as this air usually contains oil mist to lubricate pneumatic tools.

Procedure

Follow this procedure:

1	Remove the lens from the camera.
2	Use pressurized air from a compressed air canister to blow off the dust.

actoolsupply.com

actoolsupply.com

23 Technical data

For technical data, refer to the product catalog on the user documentation CD-ROM that comes with the camera.

actoolsupply.com

actoolsupply.com

24 Pin configurations

Pin configuration for USB Mini-B connector

10763203;a2

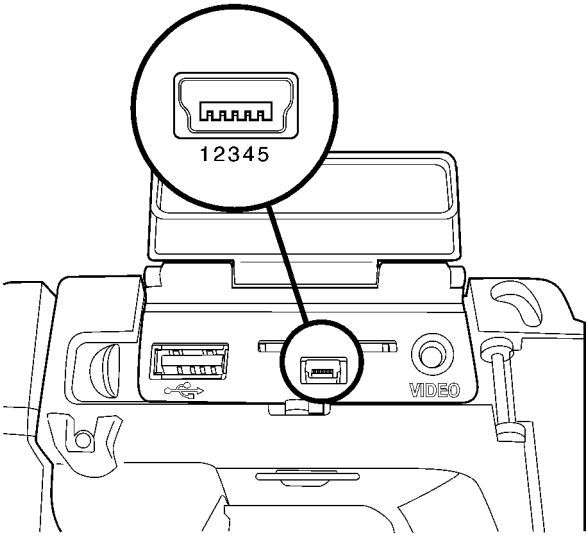

Pin	Configuration
1	+5 V (out)
2	USB –
3	USB +
4	N/C
5	Ground

actoolsupply.com

actoolsupply.com

Pin configuration for video connector

10763503;a1

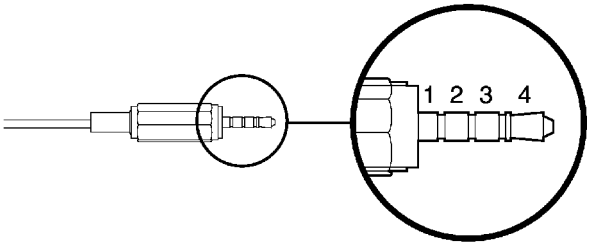

Pin	Configuration
1	Audio right
2	Ground
3	Video out
4	Audio left

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

Pin configuration for USB-A connector

10763303;a2

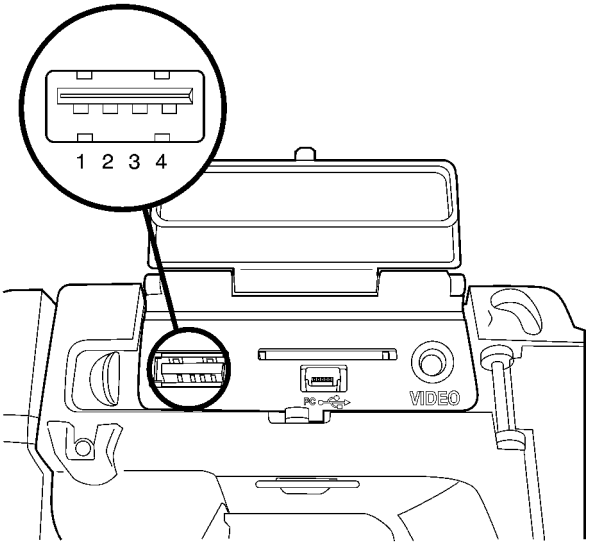

Pin	Configuration
1	+5 V (in)
2	USB –
3	USB +
4	Ground

actoolsupply.com

actoolsupply.com

Pin configuration for power connector

10763403;a1

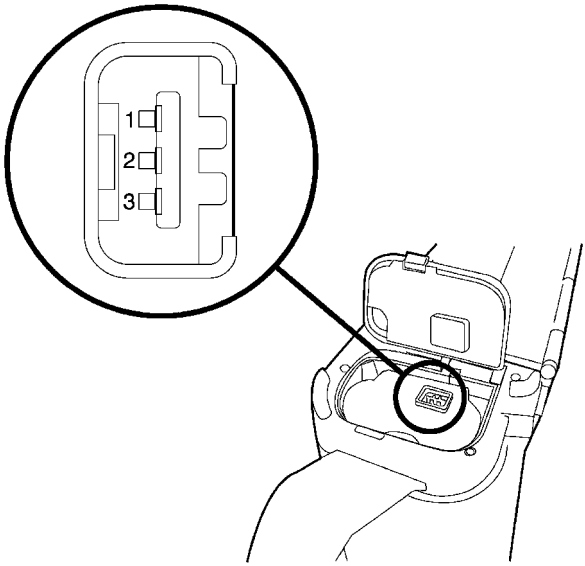

Pin	Configuration
1	+12 V
2	GND
3	GND

actoolsupply.com

25 Application examples

25.1 Moisture & water damage

General

It is often possible to detect moisture and water damage in a house by using an infrared camera. This is partly because the damaged area has a different heat conduction property and partly because it has a different thermal capacity to store heat than the surrounding material.

NOTE

Many factors can come into play as to how moisture or water damage will appear in an infrared image.

For example, heating and cooling of these parts takes place at different rates depending on the material and the time of day. For this reason, it is important that other methods are used as well to check for moisture or water damage.

Figure

The image below shows extensive water damage on an external wall where the water has penetrated the outer facing because of an incorrectly installed window ledge.

10739503;a1

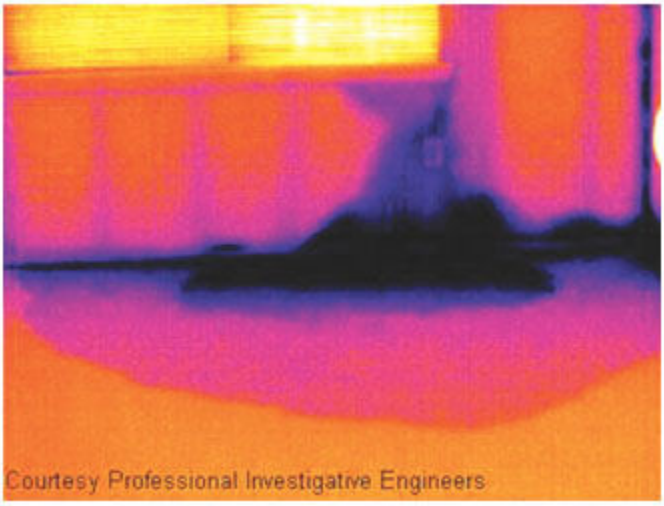

actoolsupply.com

25.2 Faulty contact in socket

General

Depending on the type of connection a socket has, an improperly connected wire can result in local temperature increase. This temperature increase is caused by the reduced contact area between the connection point of the incoming wire and the socket , and can result in an electrical fire.

NOTE

A socket's construction may differ dramatically from one manufacturer to another. For this reason, different faults in a socket can lead to the same typical appearance in an infrared image.

Local temperature increase can also result from improper contact between wire and socket, or from difference in load.

Figure

The image below shows a connection of a cable to a socket where improper contact in the connection has resulted in local temperature increase.

10739603;a1

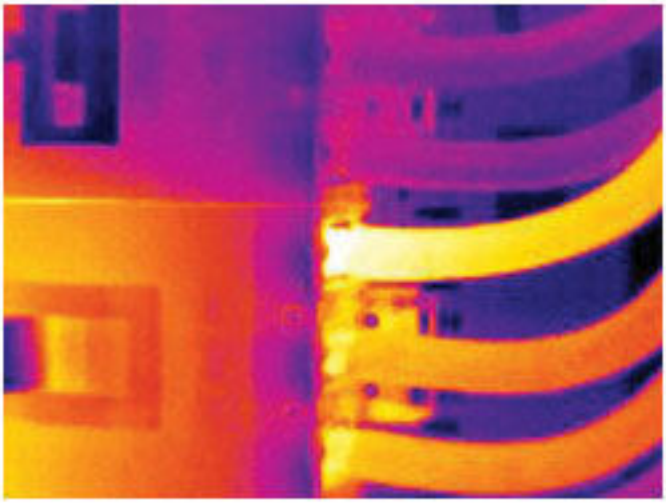

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

25.3 Oxidized socket

General

Depending on the type of socket and the environment in which the socket is installed, oxides may occur on the socket's contact surfaces. These oxides can lead to locally increased resistance when the socket is loaded, which can be seen in an infrared image as local temperature increase.

NOTE

A socket's construction may differ dramatically from one manufacturer to another. For this reason, different faults in a socket can lead to the same typical appearance in an infrared image.

Local temperature increase can also result from improper contact between a wire and socket, or from difference in load.

Figure

The image below shows a series of fuses where one fuse has a raised temperature on the contact surfaces against the fuse holder. Because of the fuse holder's blank metal, the temperature increase is not visible there, while it is visible on the fuse's ceramic material.

10739703;a1

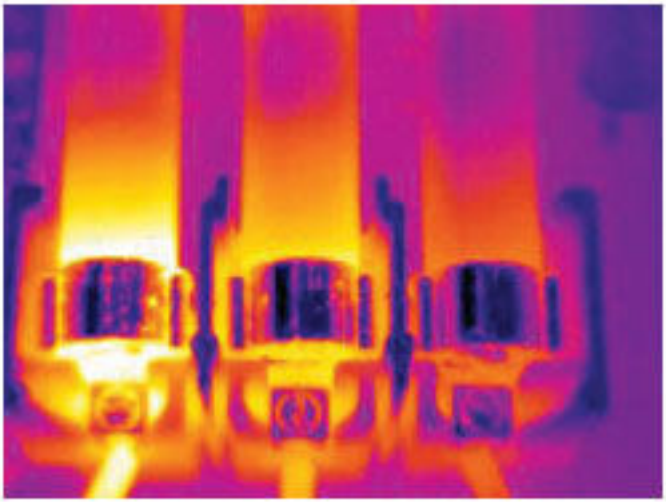

actoolsupply.com

actoolsupply.com

25.4 Insulation deficiencies

General

Insulation deficiencies may result from insulation losing volume over the course of time and thereby not entirely filling the cavity in a frame wall.

An infrared camera allows you to see these insulation deficiencies because they either have a different heat conduction property than sections with correctly installed insulation, and/or show the area where air is penetrating the frame of the building.

NOTE

When you are inspecting a building, the temperature difference between the inside and outside should be at least 10°C (18°F). Studs, water pipes, concrete columns, and similar components may resemble an insulation deficiency in an infrared image. Minor differences may also occur naturally.

Figure

In the image below, insulation in the roof framing is lacking.. Due to the absence of insulation, air has forced its way into the roof structure, which thus takes on a different characteristic appearance in the infrared image.

10739803;a1

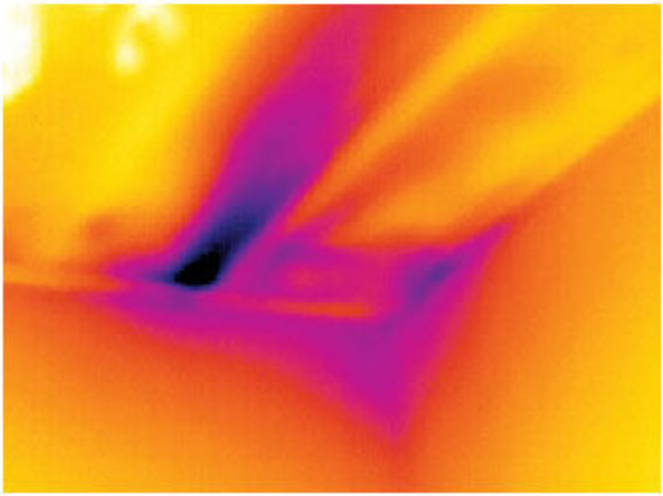

actoolsupply.com

actoolsupply.com

25.5 Draft

General

Draft can be found under baseboards, around door and window casings, and above ceiling trim. This type of draft is often possible to see with an infrared camera, as a cooler airstream cools down the surrounding surface.

NOTE

When you are investigating draft in a house, there should be sub-atmospheric pressure in the house. Close all doors, windows, and ventilation ducts, and allow the kitchen fan to run for a while before you take the infrared images.

An infrared image of draft often shows a typical stream pattern. You can see this stream pattern clearly in the picture below.

Also keep in mind that drafts can be concealed by heat from floor heating circuits.

Figure

The image below shows a ceiling hatch where faulty installation has resulted in a strong draft.

10739903;a1

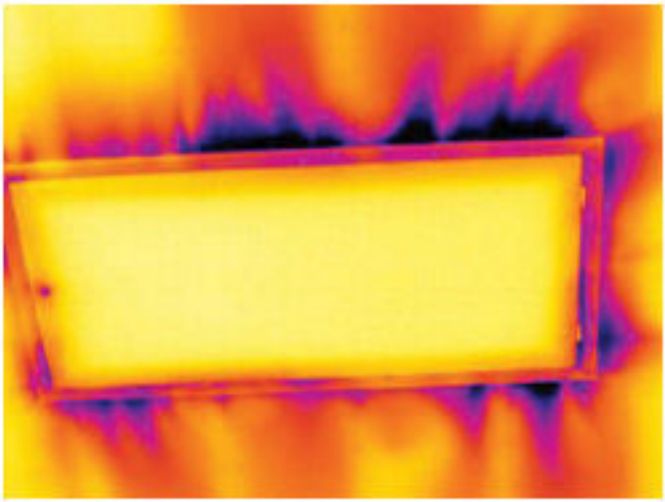

actoolsupply.com

actoolsupply.com

26 About FLIR Systems

FLIR Systems was established in 1978 to pioneer the development of high-performance infrared imaging systems, and is the world leader in the design, manufacture, and marketing of thermal imaging systems for a wide variety of commercial, industrial, and government applications. Today, FLIR Systems embraces five major companies with outstanding achievements in infrared technology since 1958—the Swedish AGEMA Infrared Systems (formerly AGA Infrared Systems), the three United States companies Indigo Systems, FSI, and Inframetrics, and the French company Cedip. In November 2007, Extech Instruments was acquired by FLIR Systems.

T638608;a1

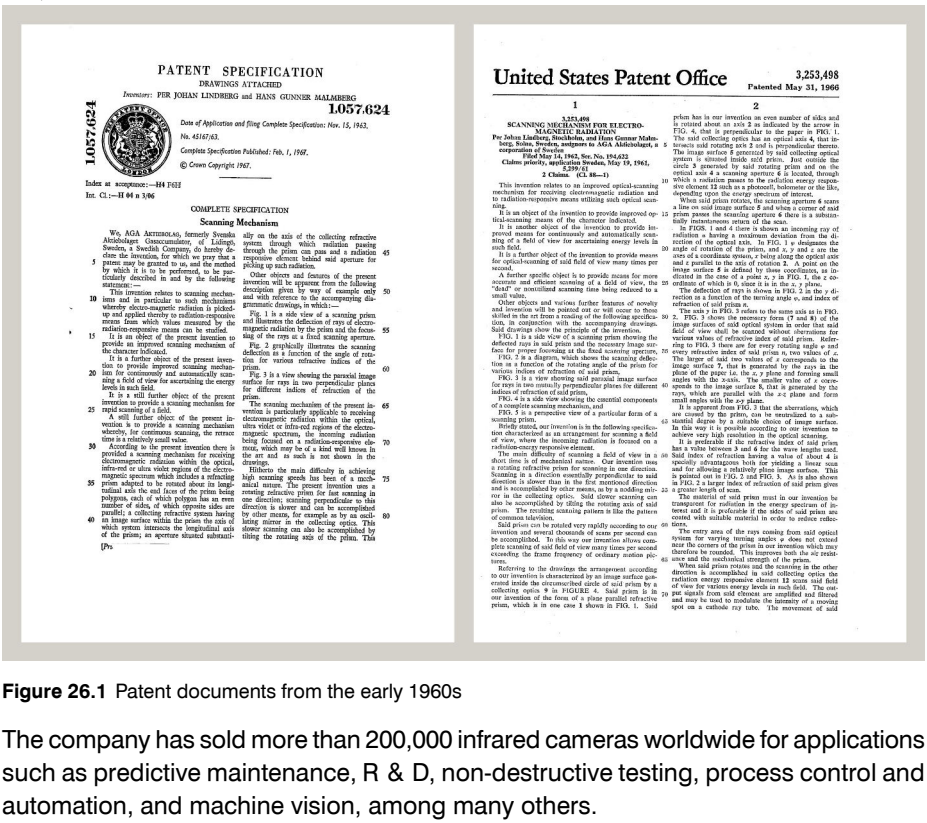

PATENT SPECIFICATION

DRAWINGS ATTACHED

Inventors: PER JOHAN LINDBERG and HANS GUNNER MALMBERG

1.057.624

1057.624

Date of Application and filing Complete Specification: Nov. 15, 1963.

No. 45167/63.

Complete Specification Published: Feb. 1, 1967.

© Crown Copyright 1967.

Index at acceptance:—H4 F6H

Int. Cl.:—H 04 n 3/06

COMPLETE SPECIFICATION

Scanning Mechanism

We, AGA AKTIEBOLAG, formerly Svenska Aktiebolaget Gasaccumulator, of Lidingö, Sweden, a Swedish Company, do hereby declare the invention, for which we pray that a patent may be granted to us, and the method by which it is to be performed, to be particularly described in and by the following statement:—

This invention relates to scanning mechanisms and in particular to such mechanisms whereby electro-magnetic radiation is picked-up and applied thereby to radiation-responsive means from which values measured by the radiation-responsive means can be studied.

It is an object of the present invention to provide an improved scanning mechanism of the character indicated.

It is a further object of the present invention to provide improved scanning mechanism for continuously and automatically scanning a field of view for ascertaining the energy levels in such field.

It is a still further object of the present invention to provide a scanning mechanism for rapid scanning of a field.

A still further object of the present invention is to provide a scanning mechanism whereby, for continuous scanning, the retrace time is a relatively small value.

According to the present invention there is provided a scanning mechanism for receiving electromagnetic radiation within the optical, infra-red or ultra violet regions of the electromagnetic spectrum which includes a refracting prism adapted to be rotated about its longitudinal axis the end faces of the prism being polygons, each of which polygon has an even number of sides, of which opposite sides are parallel; a collecting refractive system having an image surface within the prism the axis of which system intersects the longitudinally axis of the prism, an aperture situated substantially on the axis of the collecting refractive system through which radiation passing through the prism can pass and a radiation responsive element behind said aperture for picking up such radiation.

Other objects and features of the present invention will be apparent from the following description given by way of example only and with reference to the accompanying diagrammatic drawings, in which:—

Fig. 1 is a side view of a scanning prism and illustrates the deflection of rays of electromagnetic radiation by the prism and the focussing of the rays at a fixed scanning aperture.

Fig. 2 graphically illustrates the scanning deflection as a function of the angle of rotation for various refractive indices of the prism.

Fig. 3 is a view showing the parasial image surface for rays in two perpendicular planes for different indices of refraction of the prism.

The scanning mechanism of the present invention is particularly applicable to receiving electromagnetic radiation within the optical, ultra violet or infra-red regions of the electromagnetic spectrum, the incoming radiation being focused on a radiation-responsive element, which may be of a kind well known in the art and as such is not shown in the drawings.

Hitherto the main difficulty in achieving high scanning speeds has been of a mechanical nature. The present invention uses a rotating refractive prism for fast scanning in one direction; scanning perpendicular to this direction is slower and can be accomplished by other means, for example as by an oscillating mirror in the collecting optics. This slower scanning can also be accomplished by tilting the rotating axis of the prism. This

[Pto

United States Patent Office 3,253,498 Patented May 31, 1966

1 2

3,253,498
SCANNING MECHANISM FOR ELECTRO-MAGNETIC RADIATION
Per Johan Lindberg, Stockholm, and Hans Gunnar Malmberg, Solna, Sweden, assignors to AGA Aktiebolaget, a corporation of Sweden
Filed May 14, 1963, Ser. No. 280,632
Claims priority, application Sweden, May 19, 1962, 5,239/62
2 Claims. (Cl. 88—1)

This invention relates to an improved optical-scanning mechanism for receiving electromagnetic radiation and to radiation-responsive means utilizing such optical scanning.

It is an object of the invention to provide improved optical-scanning means of the character indicated.

It is another object of the invention to provide improved means for continuously and automatically scanning of a field of view for ascertaining energy levels in such field.

It is a further object of the invention to provide means for optical-scanning of said field of view many times per second.

A further specific object is to provide means for more accurate and efficient scanning of a field of view, the "dead" or nonutilized scanning time being reduced to a small value.

Other objects and various further features of novelty and invention will be pointed out or will occur to those skilled in the art from a reading of the following specification, in conjunction with the accompanying drawings. Said drawings show the principle of the invention.

FIG. 1 is a side view of a scanning prism showing the deflected rays in said prism and the necessary image surface for proper focussing at the fixed scanning aperture.

FIG. 2 is a diagram, which shows the scanning deflection as a function of the rotating angle of the prism for various indices of refraction of said prism.

FIG. 3 is a view showing said parasial image surface for rays in two mutually perpendicular planes for different indices of refraction of said prism.

FIG. 4 is a side view showing the essential components of a complete scanning mechanism, and

FIG. 5 is a perspective view of a particular form of a scanning prism.

Briefly stated, our invention is in the following specification characterized as an arrangement for scanning a field of view, where the incoming radiation is focused on a radiation-energy responsive element.

The main difficulty of scanning a field of view in a short time is of mechanical nature. Our invention uses a rotating refractive prism for scanning in one direction. Scanning in a direction essentially perpendicular to said direction is slower than in the first mentioned direction and is accomplished by other means, as by a nodding mirror in the collecting optics. Said slower scanning can also be accomplished by tilting the rotating axis of said prism. The resulting scanning pattern is like the pattern of common television.

Said prism can be rotated very rapidly according to our invention and several thousands of scans per second can be accomplished. To this way our invention allows complete scanning of said field of view many times per second exceeding the frame frequency of ordinary motion pictures.

Referring to the drawings the arrangement according to our invention is characterized by an image surface generated inside the circumscribed circle of said prism by a collecting optics 9 in FIGURE 4. Said prism in in our invention of the form of a plane parallel refractive prism, which is in one case 3 shown in FIG. 1. Said prism has in our invention an even number of sides and is rotated about an axis 2 as indicated by the arrow in FIG. 4, that is perpendicular to the paper in FIG. 1. The said collecting optics has an optical axis 4, that intersects said rotating axis 2 and is perpendicular thereto. The image surface 5 generated by said collecting optical system is situated inside said prism. Said surface the circle 3 generated by said rotating prism and the optical axis 4 a scanning aperture 6 is located, through which a radiation passes to the radiation energy responsive element 12 such as a photocell, bolometer or the like, depending upon the energy spectrum of interest.

When said prism rotates, the scanning aperture 6 scans a line on said image surface 5 and when a corner of said prism passes the scanning aperture 6 there is a substantially instantaneous return of the scan.

In FIGS. 1 and 4 there is shown an incoming ray of radiation a having a maximum deviation from the direction of the optical axis. In FIG. 1 a designates the angle of rotation of the prism, and x, y and z are the axes of a coordinate system, z being along the optical axis and z parallel to the axis of rotation 2. A point on the image surface 5 is defined by these coordinates, as indicated in the case of a point x, y in FIG. 1, the z coordinate of which is 0, since it is in the x, y plane.

The deflection of rays is shown in FIG. 2 in the y direction as a function of the moving angle a, and index of refraction of said prism n.

The axis x in FIG. 3 refers to the same axis as in FIG. 2. FIG. 3 shows the necessary form (7 and 8) of the image surfaces of said optical system in order that said field of view shall be scanned without aberrations for various values of refractive index of said prism. Referring to FIG. 3 there are for every rotating angle a and every refractive index of said prism n, two values of z. The larger of said two values of z corresponds to the image surface 7, that is generated by the rays in the plane of the paper i.e. the x, y plane and forming small angles with the x-axis. The smaller value of z corresponds to the image surface 8, that is generated by the rays, which are parallel with the x-z plane and form small angles with the x-y plane.

It is apparent from FIG. 3 that the aberrations, which are caused by the prism, can be neutralized to a substantial degree by a suitable choice of image surface. In this way it is possible according to our invention to obtain a good resolution in the optical scanning.

It is preferable if the refractive index of said prism has a value between 2 and 4 for the wave lengths used. Said index of refraction having a value of about 4 is especially advantageous both for yielding a linear scan and for allowing a relatively plane image surface. This is pointed out in FIG. 2 and FIG. 3. It is also shown in FIG. 2 a larger index of refraction of said prism gives a greater length of scan.

The material of said prism must in our invention be transparent for radiation in the energy spectrum of interest and it is preferable if the sides of said prism are coated with suitable material in order to reduce reflections.

The entry area of the rays coming from said optical system for varying turning angles a does not extend near the corners of the prism in our invention which may therefore be rounded. This improves both the air resistance and the mechanical strength of the prism.

When said prism rotates and the scanning in the other direction is accomplished in said collecting optics the radiation energy responsive element 12 scans said field of view for corresponding energy levels in such field. The output signals from said element are amplified and filtered and may be used to modulate the intensity of a moving spot on a cathode ray tube. The movement of said

Figure 26.1 Patent documents from the early 1960s

The company has sold more than 200,000 infrared cameras worldwide for applications such as predictive maintenance, R & D, non-destructive testing, process control and automation, and machine vision, among many others.

FLIR Systems has three manufacturing plants in the United States (Portland, OR, Boston, MA, Santa Barbara, CA) and one in Sweden (Stockholm). Since 2007 there is also a manufacturing plant in Tallinn, Estonia. Direct sales offices in Belgium, Brazil,

actoolsupply.com

actoolsupply.com

AC Tool Supply.com 877-207-1244 aikencolon.com

China, France, Germany, Great Britain, Hong Kong, Italy, Japan, Korea, Sweden, and the USA—together with a worldwide network of agents and distributors—support our international customer base.

FLIR Systems is at the forefront of innovation in the infrared camera industry. We anticipate market demand by constantly improving our existing cameras and developing new ones. The company has set milestones in product design and development such as the introduction of the first battery-operated portable camera for industrial inspections, and the first uncooled infrared camera, to mention just two innovations.

10722703;a2

Figure 26.2 LEFT: Thermovision® Model 661 from 1969. The camera weighed approximately 25 kg (55 lb.), the oscilloscope 20 kg (44 lb.), and the tripod 15 kg (33 lb.). The operator also needed a 220 VAC generator set, and a 10 L (2.6 US gallon) jar with liquid nitrogen. To the left of the oscilloscope the Polaroid attachment (6 kg/13 lb.) can be seen. **RIGHT:** FLIR i7 from 2009. Weight: 0.34 kg (0.75 lb.), including the battery.

FLIR Systems manufactures all vital mechanical and electronic components of the camera systems itself. From detector design and manufacturing, to lenses and system electronics, to final testing and calibration, all production steps are carried out and supervised by our own engineers. The in-depth expertise of these infrared specialists ensures the accuracy and reliability of all vital components that are assembled into your infrared camera.

26.1 More than just an infrared camera

At FLIR Systems we recognize that our job is to go beyond just producing the best infrared camera systems. We are committed to enabling all users of our infrared camera systems to work more productively by providing them with the most powerful

actoolsupply.com

actoolsupply.com

camera–software combination. Especially tailored software for predictive maintenance, R & D, and process monitoring is developed in-house. Most software is available in a wide variety of languages.

We support all our infrared cameras with a wide variety of accessories to adapt your equipment to the most demanding infrared applications.

26.2 Sharing our knowledge

Although our cameras are designed to be very user-friendly, there is a lot more to thermography than just knowing how to handle a camera. Therefore, FLIR Systems has founded the Infrared Training Center (ITC), a separate business unit, that provides certified training courses. Attending one of the ITC courses will give you a truly hands-on learning experience.

The staff of the ITC are also there to provide you with any application support you may need in putting infrared theory into practice.

26.3 Supporting our customers

FLIR Systems operates a worldwide service network to keep your camera running at all times. If you discover a problem with your camera, local service centers have all the equipment and expertise to solve it within the shortest possible time. Therefore, there is no need to send your camera to the other side of the world or to talk to someone who does not speak your language.

26.4 A few images from our facilities

10401303;a1

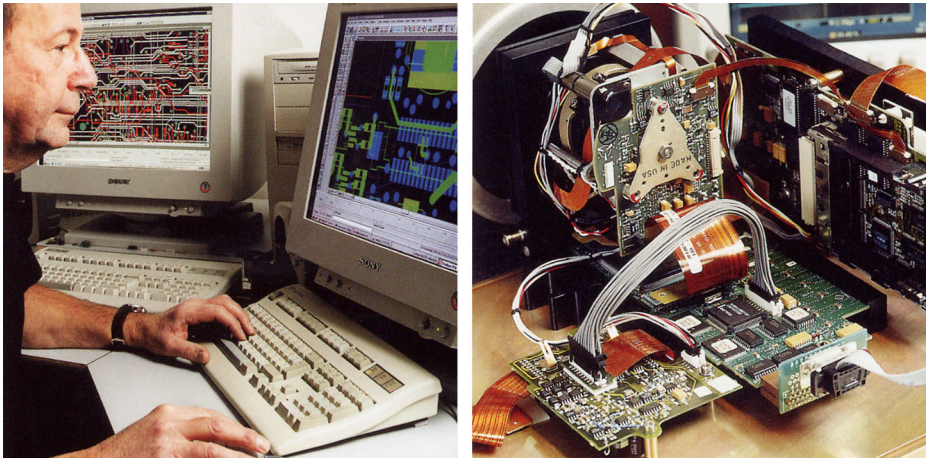

Figure 26.3 LEFT: Development of system electronics; **RIGHT:** Testing of an FPA detector

actoolsupply.com

actoolsupply.com

10401403;a1

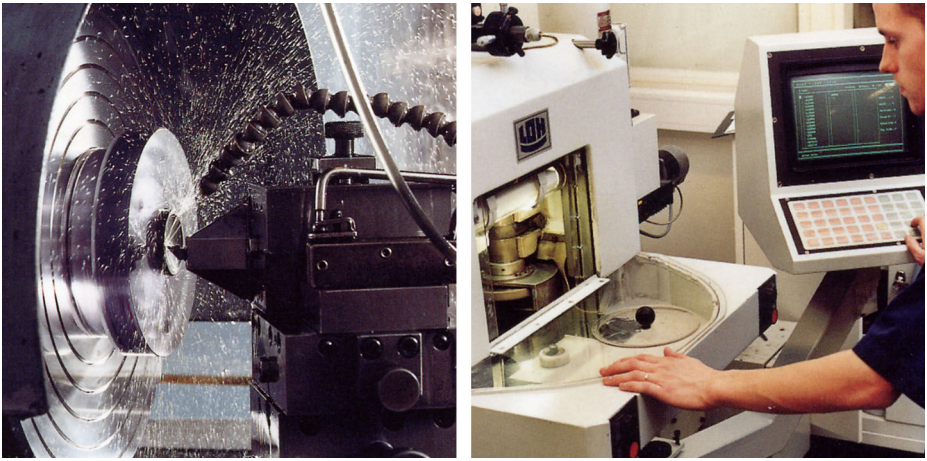

Figure 26.4 LEFT: Diamond turning machine; **RIGHT:** Lens polishing

10401503;a1

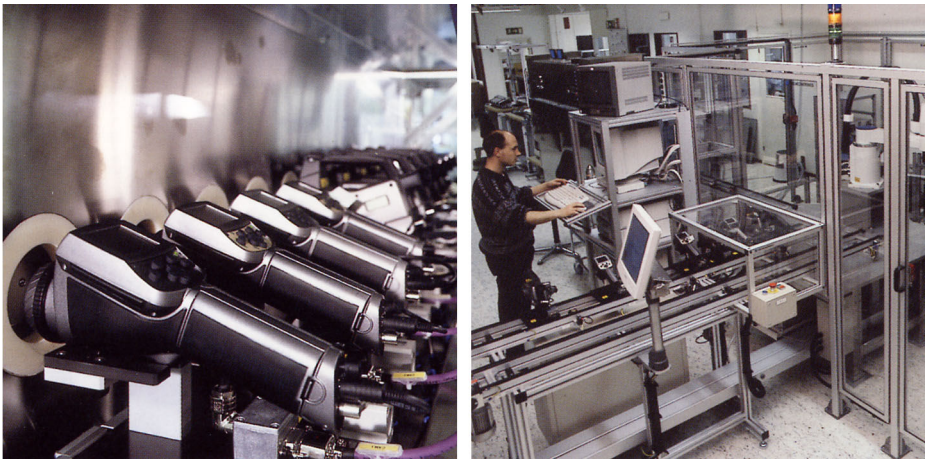

Figure 26.5 LEFT: Testing of infrared cameras in the climatic chamber; **RIGHT:** Robot used for camera testing and calibration

actoolsupply.com

actoolsupply.com

27 Glossary

Term or expression	Explanation
absorption (absorption factor)	The amount of radiation absorbed by an object relative to the received radiation. A number between 0 and 1.
atmosphere	The gases between the object being measured and the camera, normally air.
autoadjust	A function making a camera perform an internal image correction.
autopalette	The IR image is shown with an uneven spread of colors, displaying cold objects as well as hot ones at the same time.
blackbody	Totally non-reflective object. All its radiation is due to its own temperature.
blackbody radiator	An IR radiating equipment with blackbody properties used to calibrate IR cameras.
calculated atmospheric transmission	A transmission value computed from the temperature, the relative humidity of air and the distance to the object.
cavity radiator	A bottle shaped radiator with an absorbing inside, viewed through the bottleneck.
color temperature	The temperature for which the color of a blackbody matches a specific color.
conduction	The process that makes heat diffuse into a material.
continuous adjust	A function that adjusts the image. The function works all the time, continuously adjusting brightness and contrast according to the image content.
convection	Convection is a heat transfer mode where a fluid is brought into motion, either by gravity or another force, thereby transferring heat from one place to another.
dual isotherm	An isotherm with two color bands, instead of one.
emissivity (emissivity factor)	The amount of radiation coming from an object, compared to that of a blackbody. A number between 0 and 1.
emittance	Amount of energy emitted from an object per unit of time and area (W/m^2)
environment	Objects and gases that emit radiation towards the object being measured.
estimated atmospheric transmission	A transmission value, supplied by a user, replacing a calculated one

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

Term or expression	Explanation
external optics	Extra lenses, filters, heat shields etc. that can be put between the camera and the object being measured.
filter	A material transparent only to some of the infrared wavelengths.
FOV	Field of view: The horizontal angle that can be viewed through an IR lens.
FPA	Focal plane array: A type of IR detector.
graybody	An object that emits a fixed fraction of the amount of energy of a blackbody for each wavelength.
IFOV	Instantaneous field of view: A measure of the geometrical resolution of an IR camera.
image correction (internal or external)	A way of compensating for sensitivity differences in various parts of live images and also of stabilizing the camera.
infrared	Non-visible radiation, having a wavelength from about 2–13 µm.
IR	infrared
isotherm	A function highlighting those parts of an image that fall above, below or between one or more temperature intervals.
isothermal cavity	A bottle-shaped radiator with a uniform temperature viewed through the bottleneck.
Laser LocatIR	An electrically powered light source on the camera that emits laser radiation in a thin, concentrated beam to point at certain parts of the object in front of the camera.
laser pointer	An electrically powered light source on the camera that emits laser radiation in a thin, concentrated beam to point at certain parts of the object in front of the camera.
level	The center value of the temperature scale, usually expressed as a signal value.
manual adjust	A way to adjust the image by manually changing certain parameters.
NETD	Noise equivalent temperature difference. A measure of the image noise level of an IR camera.
noise	Undesired small disturbance in the infrared image
object parameters	A set of values describing the circumstances under which the measurement of an object was made, and the object itself (such as emissivity, reflected apparent temperature, distance etc.)
object signal	A non-calibrated value related to the amount of radiation received by the camera from the object.

actoolsupply.com

actoolsupply.com

Term or expression	Explanation
palette	The set of colors used to display an IR image.
pixel	Stands for *picture element*. One single spot in an image.
radiance	Amount of energy emitted from an object per unit of time, area and angle ($W/m^2/sr$)
radiant power	Amount of energy emitted from an object per unit of time (W)
radiation	The process by which electromagnetic energy, is emitted by an object or a gas.
radiator	A piece of IR radiating equipment.
range	The current overall temperature measurement limitation of an IR camera. Cameras can have several ranges. Expressed as two blackbody temperatures that limit the current calibration.
reference temperature	A temperature which the ordinary measured values can be compared with.
reflection	The amount of radiation reflected by an object relative to the received radiation. A number between 0 and 1.
relative humidity	Relative humidity represents the ratio between the current water vapour mass in the air and the maximum it may contain in saturation conditions.
saturation color	The areas that contain temperatures outside the present level/span settings are colored with the saturation colors. The saturation colors contain an ‘overflow’ color and an ‘underflow’ color. There is also a third red saturation color that marks everything saturated by the detector indicating that the range should probably be changed.
span	The interval of the temperature scale, usually expressed as a signal value.
spectral (radiant) emittance	Amount of energy emitted from an object per unit of time, area and wavelength ($W/m^2/\mu m$)
temperature difference, or difference of temperature.	A value which is the result of a subtraction between two temperature values.
temperature range	The current overall temperature measurement limitation of an IR camera. Cameras can have several ranges. Expressed as two blackbody temperatures that limit the current calibration.
temperature scale	The way in which an IR image currently is displayed. Expressed as two temperature values limiting the colors.
thermogram	infrared image

actoolsupply.com

actoolsupply.com

Term or expression	Explanation
transmission (or transmittance) factor	Gases and materials can be more or less transparent. Transmission is the amount of IR radiation passing through them. A number between 0 and 1.
transparent isotherm	An isotherm showing a linear spread of colors, instead of covering the highlighted parts of the image.
visual	Refers to the video mode of a IR camera, as opposed to the normal, thermographic mode. When a camera is in video mode it captures ordinary video images, while thermographic images are captured when the camera is in IR mode.

actoolsupply.com

actoolsupply.com

28 Thermographic measurement techniques

28.1 Introduction

An infrared camera measures and images the emitted infrared radiation from an object. The fact that radiation is a function of object surface temperature makes it possible for the camera to calculate and display this temperature.

However, the radiation measured by the camera does not only depend on the temperature of the object but is also a function of the emissivity. Radiation also originates from the surroundings and is reflected in the object. The radiation from the object and the reflected radiation will also be influenced by the absorption of the atmosphere.

To measure temperature accurately, it is therefore necessary to compensate for the effects of a number of different radiation sources. This is done on-line automatically by the camera. The following object parameters must, however, be supplied for the camera:

- The emissivity of the object
- The reflected apparent temperature
- The distance between the object and the camera
- The relative humidity
- Temperature of the atmosphere

28.2 Emissivity

The most important object parameter to set correctly is the emissivity which, in short, is a measure of how much radiation is emitted from the object, compared to that from a perfect blackbody of the same temperature.

Normally, object materials and surface treatments exhibit emissivity ranging from approximately 0.1 to 0.95. A highly polished (mirror) surface falls below 0.1, while an oxidized or painted surface has a higher emissivity. Oil-based paint, regardless of color in the visible spectrum, has an emissivity over 0.9 in the infrared. Human skin exhibits an emissivity 0.97 to 0.98.

Non-oxidized metals represent an extreme case of perfect opacity and high reflexivity, which does not vary greatly with wavelength. Consequently, the emissivity of metals is low – only increasing with temperature. For non-metals, emissivity tends to be high, and decreases with temperature.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

28.2.1 Finding the emissivity of a sample

28.2.1.1 Step 1: Determining reflected apparent temperature

Use one of the following two methods to determine reflected apparent temperature:

28.2.1.1.1 Method 1: Direct method

1	Look for possible reflection sources, considering that the incident angle = reflection angle (a = b). 10588903;a1 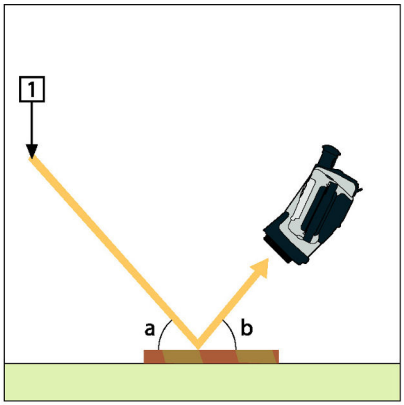 **Figure 28.1** 1 = Reflection source
2	If the reflection source is a spot source, modify the source by obstructing it using a piece if cardboard. 10589103;a2 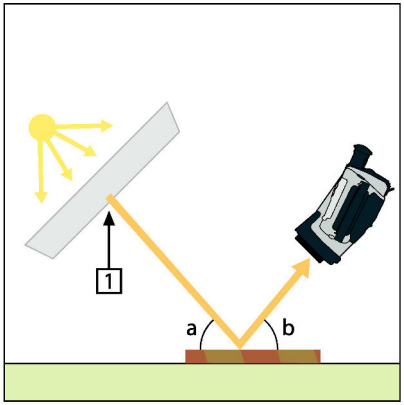 **Figure 28.2** 1 = Reflection source

actoolsupply.com

actoolsupply.com

3	Measure the radiation intensity (= apparent temperature) from the reflecting source using the following settings: ▪ Emissivity: 1.0 ▪ D_{obj}: 0 You can measure the radiation intensity using one of the following two methods: 10589003;a2 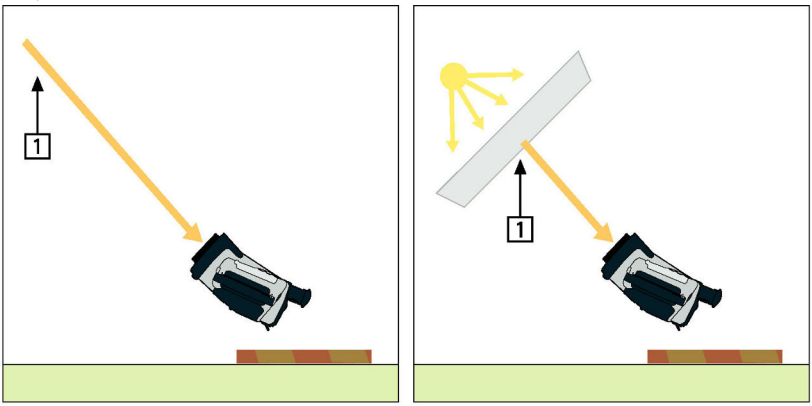 **Figure 28.3** 1 = Reflection source

Note: Using a thermocouple to measure reflected apparent temperature is not recommended for two important reasons:

- A thermocouple does not measure radiation intensity
- A thermocouple requires a very good thermal contact to the surface, usually by gluing and covering the sensor by a thermal isolator.

28.2.1.1.2 Method 2: Reflector method

1	Crumble up a large piece of aluminum foil.
2	Uncrumble the aluminum foil and attach it to a piece of cardboard of the same size.
3	Put the piece of cardboard in front of the object you want to measure. Make sure that the side with aluminum foil points to the camera.
4	Set the emissivity to 1.0.

actoolsupply.com

actoolsupply.com

5	Measure the apparent temperature of the aluminum foil and write it down.

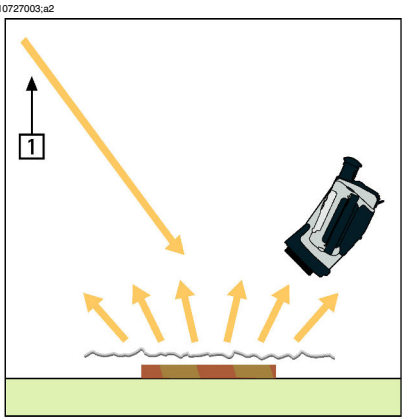

Figure 28.4 Measuring the apparent temperature of the aluminum foil

28.2.1.2 Step 2: Determining the emissivity

1	Select a place to put the sample.
2	Determine and set reflected apparent temperature according to the previous procedure.
3	Put a piece of electrical tape with known high emissivity on the sample.
4	Heat the sample at least 20 K above room temperature. Heating must be reasonably even.
5	Focus and auto-adjust the camera, and freeze the image.
6	Adjust **Level** and **Span** for best image brightness and contrast.
7	Set emissivity to that of the tape (usually 0.97).
8	Measure the temperature of the tape using one of the following measurement functions: ▪ **Isotherm** (helps you to determine both the temperature and how evenly you have heated the sample) ▪ **Spot** (simpler) ▪ **Box Avg** (good for surfaces with varying emissivity).
9	Write down the temperature.
10	Move your measurement function to the sample surface.
11	Change the emissivity setting until you read the same temperature as your previous measurement.
12	Write down the emissivity.

Note:

actoolsupply.com

actoolsupply.com

- Avoid forced convection
- Look for a thermally stable surrounding that will not generate spot reflections
- Use high quality tape that you know is not transparent, and has a high emissivity you are certain of
- This method assumes that the temperature of your tape and the sample surface are the same. If they are not, your emissivity measurement will be wrong.

28.3 Reflected apparent temperature

This parameter is used to compensate for the radiation reflected in the object. If the emissivity is low and the object temperature relatively far from that of the reflected it will be important to set and compensate for the reflected apparent temperature correctly.

28.4 Distance

The distance is the distance between the object and the front lens of the camera. This parameter is used to compensate for the following two facts:

- That radiation from the target is absorbed by the athmosphere between the object and the camera.
- That radiation from the atmosphere itself is detected by the camera.

28.5 Relative humidity

The camera can also compensate for the fact that the transmittance is also dependent on the relative humidity of the atmosphere. To do this set the relative humidity to the correct value. For short distances and normal humidity the relative humidity can normally be left at a default value of 50%.

28.6 Other parameters

In addition, some cameras and analysis programs from FLIR Systems allow you to compensate for the following parameters:

- Atmospheric temperature – *i.e.* the temperature of the atmosphere between the camera and the target
- External optics temperature – *i.e.* the temperature of any external lenses or windows used in front of the camera
- External optics transmittance – *i.e.* the transmission of any external lenses or windows used in front of the camera

actoolsupply.com

AC Tool Supply.com
877-207-1244
aikencolon.com

29 History of infrared technology

Before the year 1800, the existence of the infrared portion of the electromagnetic spectrum wasn't even suspected. The original significance of the infrared spectrum, or simply 'the infrared' as it is often called, as a form of heat radiation is perhaps less obvious today than it was at the time of its discovery by Herschel in 1800.

10398703;a1



Figure 29.1 Sir William Herschel (1738–1822)

The discovery was made accidentally during the search for a new optical material. Sir William Herschel – Royal Astronomer to King George III of England, and already famous for his discovery of the planet Uranus – was searching for an optical filter material to reduce the brightness of the sun's image in telescopes during solar observations. While testing different samples of colored glass which gave similar reductions in brightness he was intrigued to find that some of the samples passed very little of the sun's heat, while others passed so much heat that he risked eye damage after only a few seconds' observation.

Herschel was soon convinced of the necessity of setting up a systematic experiment, with the objective of finding a single material that would give the desired reduction in brightness as well as the maximum reduction in heat. He began the experiment by actually repeating Newton's prism experiment, but looking for the heating effect rather than the visual distribution of intensity in the spectrum. He first blackened the bulb of a sensitive mercury-in-glass thermometer with ink, and with this as his radiation detector he proceeded to test the heating effect of the various colors of the spectrum formed on the top of a table by passing sunlight through a glass prism. Other thermometers, placed outside the sun's rays, served as controls.

As the blackened thermometer was moved slowly along the colors of the spectrum, the temperature readings showed a steady increase from the violet end to the red end. This was not entirely unexpected, since the Italian researcher, Landriani, in a similar experiment in 1777 had observed much the same effect. It was Herschel,

actoolsupply.com

however, who was the first to recognize that there must be a point where the heating effect reaches a maximum, and that measurements confined to the visible portion of the spectrum failed to locate this point.

10398903;a1

Figure 29.2 Marsilio Landriani (1746–1815)

Moving the thermometer into the dark region beyond the red end of the spectrum, Herschel confirmed that the heating continued to increase. The maximum point, when he found it, lay well beyond the red end – in what is known today as the 'infrared wavelengths'.

When Herschel revealed his discovery, he referred to this new portion of the electromagnetic spectrum as the 'thermometrical spectrum'. The radiation itself he sometimes referred to as 'dark heat', or simply 'the invisible rays'. Ironically, and contrary to popular opinion, it wasn't Herschel who originated the term 'infrared'. The word only began to appear in print around 75 years later, and it is still unclear who should receive credit as the originator.

Herschel's use of glass in the prism of his original experiment led to some early controversies with his contemporaries about the actual existence of the infrared wavelengths. Different investigators, in attempting to confirm his work, used various types of glass indiscriminately, having different transparencies in the infrared. Through his later experiments, Herschel was aware of the limited transparency of glass to the newly-discovered thermal radiation, and he was forced to conclude that optics for the infrared would probably be doomed to the use of reflective elements exclusively (i.e. plane and curved mirrors). Fortunately, this proved to be true only until 1830, when the Italian investigator, Melloni, made his great discovery that naturally occurring rock salt (NaCl) – which was available in large enough natural crystals to be made into lenses and prisms – is remarkably transparent to the infrared. The result was that rock salt became the principal infrared optical material, and remained so for the next hundred years, until the art of synthetic crystal growing was mastered in the 1930's.

actoolsupply.com

actoolsupply.com

10399103;a1

Figure 29.3 Macedonio Melloni (1798–1854)

Thermometers, as radiation detectors, remained unchallenged until 1829, the year Nobili invented the thermocouple. (Herschel's own thermometer could be read to 0.2 °C (0.036 °F), and later models were able to be read to 0.05 °C (0.09 °F)). Then a breakthrough occurred; Melloni connected a number of thermocouples in series to form the first thermopile. The new device was at least 40 times as sensitive as the best thermometer of the day for detecting heat radiation – capable of detecting the heat from a person standing three meters away.

The first so-called 'heat-picture' became possible in 1840, the result of work by Sir John Herschel, son of the discoverer of the infrared and a famous astronomer in his own right. Based upon the differential evaporation of a thin film of oil when exposed to a heat pattern focused upon it, the thermal image could be seen by reflected light where the interference effects of the oil film made the image visible to the eye. Sir John also managed to obtain a primitive record of the thermal image on paper, which he called a 'thermograph'.

10399003;a2

Figure 29.4 Samuel P. Langley (1834–1906)

actoolsupply.com

actoolsupply.com

The improvement of infrared-detector sensitivity progressed slowly. Another major breakthrough, made by Langley in 1880, was the invention of the bolometer. This consisted of a thin blackened strip of platinum connected in one arm of a Wheatstone bridge circuit upon which the infrared radiation was focused and to which a sensitive galvanometer responded. This instrument is said to have been able to detect the heat from a cow at a distance of 400 meters.

An English scientist, Sir James Dewar, first introduced the use of liquefied gases as cooling agents (such as liquid nitrogen with a temperature of -196 °C (-320.8 °F)) in low temperature research. In 1892 he invented a unique vacuum insulating container in which it is possible to store liquefied gases for entire days. The common 'thermos bottle', used for storing hot and cold drinks, is based upon his invention.

Between the years 1900 and 1920, the inventors of the world 'discovered' the infrared. Many patents were issued for devices to detect personnel, artillery, aircraft, ships – and even icebergs. The first operating systems, in the modern sense, began to be developed during the 1914–18 war, when both sides had research programs devoted to the military exploitation of the infrared. These programs included experimental systems for enemy intrusion/detection, remote temperature sensing, secure communications, and 'flying torpedo' guidance. An infrared search system tested during this period was able to detect an approaching airplane at a distance of 1.5 km (0.94 miles), or a person more than 300 meters (984 ft.) away.

The most sensitive systems up to this time were all based upon variations of the bolometer idea, but the period between the two wars saw the development of two revolutionary new infrared detectors: the image converter and the photon detector. At first, the image converter received the greatest attention by the military, because it enabled an observer for the first time in history to literally 'see in the dark'. However, the sensitivity of the image converter was limited to the near infrared wavelengths, and the most interesting military targets (i.e. enemy soldiers) had to be illuminated by infrared search beams. Since this involved the risk of giving away the observer's position to a similarly-equipped enemy observer, it is understandable that military interest in the image converter eventually faded.

The tactical military disadvantages of so-called 'active' (i.e. search beam-equipped) thermal imaging systems provided impetus following the 1939–45 war for extensive secret military infrared-research programs into the possibilities of developing 'passive' (no search beam) systems around the extremely sensitive photon detector. During this period, military secrecy regulations completely prevented disclosure of the status of infrared-imaging technology. This secrecy only began to be lifted in the middle of the 1950's, and from that time adequate thermal-imaging devices finally began to be available to civilian science and industry.

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

30 Theory of thermography

30.1 Introduction

The subjects of infrared radiation and the related technique of thermography are still new to many who will use an infrared camera. In this section the theory behind thermography will be given.

30.2 The electromagnetic spectrum

The electromagnetic spectrum is divided arbitrarily into a number of wavelength regions, called *bands*, distinguished by the methods used to produce and detect the radiation. There is no fundamental difference between radiation in the different bands of the electromagnetic spectrum. They are all governed by the same laws and the only differences are those due to differences in wavelength.

10067803;a1

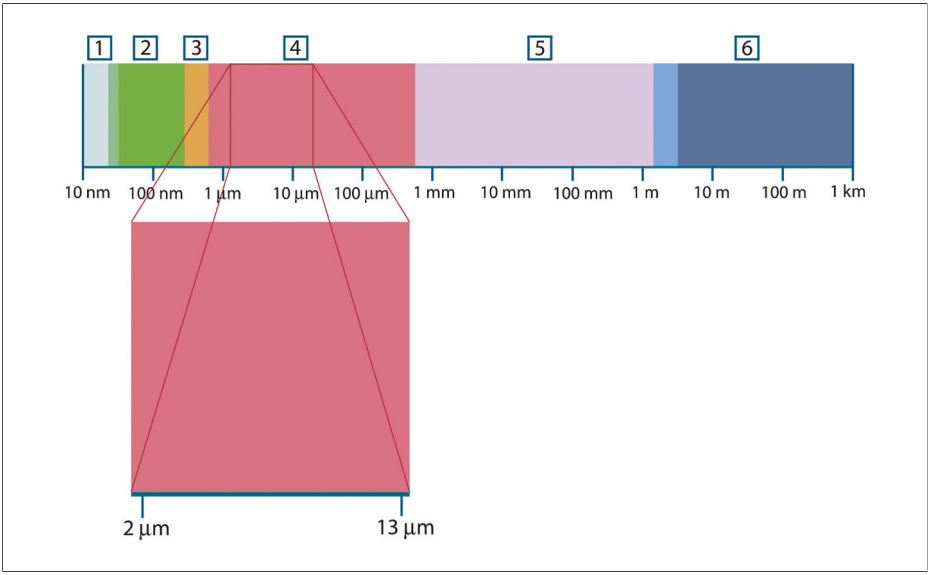

Figure 30.1 The electromagnetic spectrum. **1:** X-ray; **2:** UV; **3:** Visible; **4:** IR; **5:** Microwaves; **6:** Radiowaves.

Thermography makes use of the infrared spectral band. At the short-wavelength end the boundary lies at the limit of visual perception, in the deep red. At the long-wavelength end it merges with the microwave radio wavelengths, in the millimeter range.

The infrared band is often further subdivided into four smaller bands, the boundaries of which are also arbitrarily chosen. They include: the *near infrared* (0.75–3 µm), the *middle infrared* (3–6 µm), the *far infrared* (6–15 µm) and the *extreme infrared* (15–100

actoolsupply.com

actoolsupply.com

µm). Although the wavelengths are given in µm (micrometers), other units are often still used to measure wavelength in this spectral region, *e.g.* nanometer (nm) and Ångström (Å).

The relationships between the different wavelength measurements is:

$$10\ 000\ \text{Å} = 1\ 000\ \text{nm} = 1\ \mu = 1\ \mu\text{m}$$

30.3 Blackbody radiation

A blackbody is defined as an object which absorbs all radiation that impinges on it at any wavelength. The apparent misnomer *black* relating to an object emitting radiation is explained by Kirchhoff's Law (after *Gustav Robert Kirchhoff*, 1824–1887), which states that a body capable of absorbing all radiation at any wavelength is equally capable in the emission of radiation.

10398803;a1

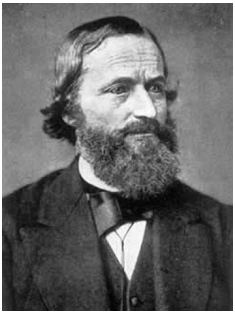

Figure 30.2 Gustav Robert Kirchhoff (1824–1887)

The construction of a blackbody source is, in principle, very simple. The radiation characteristics of an aperture in an isotherm cavity made of an opaque absorbing material represents almost exactly the properties of a blackbody. A practical application of the principle to the construction of a perfect absorber of radiation consists of a box that is light tight except for an aperture in one of the sides. Any radiation which then enters the hole is scattered and absorbed by repeated reflections so only an infinitesimal fraction can possibly escape. The blackness which is obtained at the aperture is nearly equal to a blackbody and almost perfect for all wavelengths.

By providing such an isothermal cavity with a suitable heater it becomes what is termed a *cavity radiator*. An isothermal cavity heated to a uniform temperature generates blackbody radiation, the characteristics of which are determined solely by the temperature of the cavity. Such cavity radiators are commonly used as sources of radiation in temperature reference standards in the laboratory for calibrating thermographic instruments, such as a FLIR Systems camera for example.

actoolsupply.com

actoolsupply.com

If the temperature of blackbody radiation increases to more than 525°C (977°F), the source begins to be visible so that it appears to the eye no longer black. This is the incipient red heat temperature of the radiator, which then becomes orange or yellow as the temperature increases further. In fact, the definition of the so-called *color temperature* of an object is the temperature to which a blackbody would have to be heated to have the same appearance.

Now consider three expressions that describe the radiation emitted from a blackbody.

30.3.1 Planck's law

10399203;a1

Figure 30.3 Max Planck (1858–1947)

Max Planck (1858–1947) was able to describe the spectral distribution of the radiation from a blackbody by means of the following formula:

$$W_{\lambda b} = \frac{2\pi hc^2}{\lambda^5\left(e^{hc/\lambda kT} - 1\right)} \times 10^{-6}[Watt/m^2, \mu m]$$

where:

$W_{\lambda b}$	Blackbody spectral radiant emittance at wavelength λ.
c	Velocity of light = 3×10^8 m/s
h	Planck's constant = 6.6×10^{-34} Joule sec.
k	Boltzmann's constant = 1.4×10^{-23} Joule/K.
T	Absolute temperature (K) of a blackbody.
λ	Wavelength (μm).

actoolsupply.com

actoolsupply.com

➲ The factor 10^{-6} is used since spectral emittance in the curves is expressed in Watt/m^2, µm.

Planck's formula, when plotted graphically for various temperatures, produces a family of curves. Following any particular Planck curve, the spectral emittance is zero at $\lambda = 0$, then increases rapidly to a maximum at a wavelength λ_{max} and after passing it approaches zero again at very long wavelengths. The higher the temperature, the shorter the wavelength at which maximum occurs.

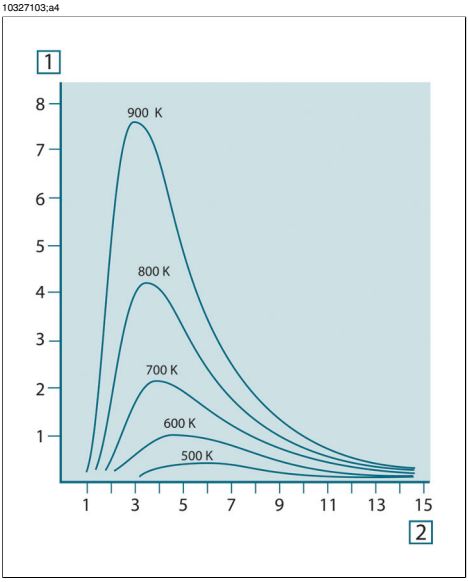

Figure 30.4 Blackbody spectral radiant emittance according to Planck's law, plotted for various absolute temperatures. **1:** Spectral radiant emittance (W/cm^2 × 10^3(µm)); **2:** Wavelength (µm)

30.3.2 Wien's displacement law

By differentiating Planck's formula with respect to λ, and finding the maximum, we have:

$$\lambda_{max} = \frac{2898}{T}[\mu m]$$

This is Wien's formula (after *Wilhelm Wien*, 1864–1928), which expresses mathematically the common observation that colors vary from red to orange or yellow as the temperature of a thermal radiator increases. The wavelength of the color is the same as the wavelength calculated for λ_{max}. A good approximation of the value of λ_{max} for a given blackbody temperature is obtained by applying the rule-of-thumb 3 000/T

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

µm. Thus, a very hot star such as Sirius (11 000 K), emitting bluish-white light, radiates with the peak of spectral radiant emittance occurring within the invisible ultraviolet spectrum, at wavelength 0.27 µm.

10399403;a1

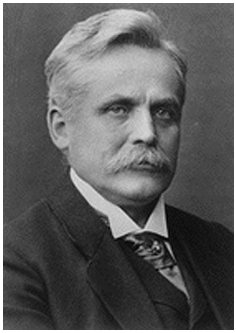

Figure 30.5 Wilhelm Wien (1864–1928)

The sun (approx. 6 000 K) emits yellow light, peaking at about 0.5 µm in the middle of the visible light spectrum.

At room temperature (300 K) the peak of radiant emittance lies at 9.7 µm, in the far infrared, while at the temperature of liquid nitrogen (77 K) the maximum of the almost insignificant amount of radiant emittance occurs at 38 µm, in the extreme infrared wavelengths.

actoolsupply.com

actoolsupply.com

10327203;a4

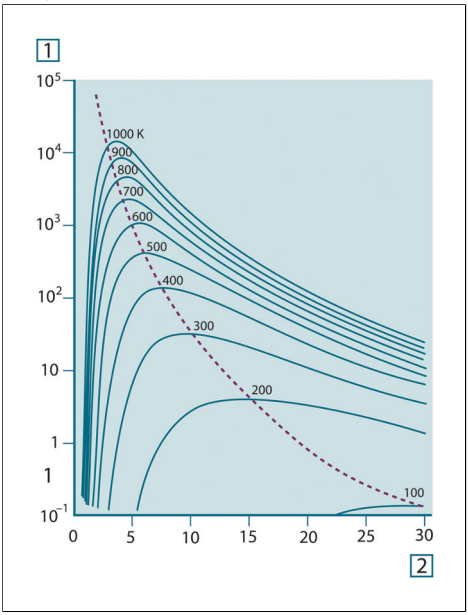

Figure 30.6 Planckian curves plotted on semi-log scales from 100 K to 1000 K. The dotted line represents the locus of maximum radiant emittance at each temperature as described by Wien's displacement law. **1:** Spectral radiant emittance (W/cm^2 (µm)); **2:** Wavelength (µm).

30.3.3 Stefan-Boltzmann's law

By integrating Planck's formula from $\lambda = 0$ to $\lambda = \infty$, we obtain the total radiant emittance (W_b) of a blackbody:

$$W_b = \sigma T^4 \ [\mathrm{Watt/m^2}]$$

This is the Stefan-Boltzmann formula (after *Josef Stefan*, 1835–1893, and *Ludwig Boltzmann*, 1844–1906), which states that the total emissive power of a blackbody is proportional to the fourth power of its absolute temperature. Graphically, W_b represents the area below the Planck curve for a particular temperature. It can be shown that the radiant emittance in the interval $\lambda = 0$ to λ_{max} is only 25% of the total, which represents about the amount of the sun's radiation which lies inside the visible light spectrum.

actoolsupply.com

actoolsupply.com

10399303;a1

Figure 30.7 Josef Stefan (1835–1893), and Ludwig Boltzmann (1844–1906)

Using the Stefan-Boltzmann formula to calculate the power radiated by the human body, at a temperature of 300 K and an external surface area of approx. 2 m^2, we obtain 1 kW. This power loss could not be sustained if it were not for the compensating absorption of radiation from surrounding surfaces, at room temperatures which do not vary too drastically from the temperature of the body – or, of course, the addition of clothing.

30.3.4 Non-blackbody emitters

So far, only blackbody radiators and blackbody radiation have been discussed. However, real objects almost never comply with these laws over an extended wavelength region – although they may approach the blackbody behavior in certain spectral intervals. For example, a certain type of white paint may appear perfectly *white* in the visible light spectrum, but becomes distinctly *gray* at about 2 µm, and beyond 3 µm it is almost *black*.

There are three processes which can occur that prevent a real object from acting like a blackbody: a fraction of the incident radiation α may be absorbed, a fraction ρ may be reflected, and a fraction τ may be transmitted. Since all of these factors are more or less wavelength dependent, the subscript λ is used to imply the spectral dependence of their definitions. Thus:

- The spectral absorptance α_λ = the ratio of the spectral radiant power absorbed by an object to that incident upon it.
- The spectral reflectance ρ_λ = the ratio of the spectral radiant power reflected by an object to that incident upon it.
- The spectral transmittance τ_λ = the ratio of the spectral radiant power transmitted through an object to that incident upon it.

The sum of these three factors must always add up to the whole at any wavelength, so we have the relation:

$$\alpha_\lambda + \rho_\lambda + \tau_\lambda = 1$$

actoolsupply.com

actoolsupply.com

For opaque materials $\tau_\lambda = 0$ and the relation simplifies to:

$$\alpha_\lambda + \rho_\lambda = 1$$

Another factor, called the emissivity, is required to describe the fraction ε of the radiant emittance of a blackbody produced by an object at a specific temperature. Thus, we have the definition:

The spectral emissivity ε_λ= the ratio of the spectral radiant power from an object to that from a blackbody at the same temperature and wavelength.

Expressed mathematically, this can be written as the ratio of the spectral emittance of the object to that of a blackbody as follows:

$$\varepsilon_\lambda = \frac{W_{\lambda o}}{W_{\lambda b}}$$

Generally speaking, there are three types of radiation source, distinguished by the ways in which the spectral emittance of each varies with wavelength.

- A blackbody, for which $\varepsilon_\lambda = \varepsilon = 1$
- A graybody, for which $\varepsilon_\lambda = \varepsilon$ = constant less than 1
- A selective radiator, for which ε varies with wavelength

According to Kirchhoff's law, for any material the spectral emissivity and spectral absorptance of a body are equal at any specified temperature and wavelength. That is:

$$\varepsilon_\lambda = \alpha_\lambda$$

From this we obtain, for an opaque material (since $\alpha_\lambda + \rho_\lambda = 1$):

$$\varepsilon_\lambda + \rho_\lambda = 1$$

For highly polished materials ε_λ approaches zero, so that for a perfectly reflecting material (*i.e.* a perfect mirror) we have:

$$\rho_\lambda = 1$$

For a graybody radiator, the Stefan-Boltzmann formula becomes:

$$W = \varepsilon \sigma T^4 \ [\mathrm{Watt/m^2}]$$

This states that the total emissive power of a graybody is the same as a blackbody at the same temperature reduced in proportion to the value of ε from the graybody.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM
877-207-1244
aikencolon.com

10401203;a2

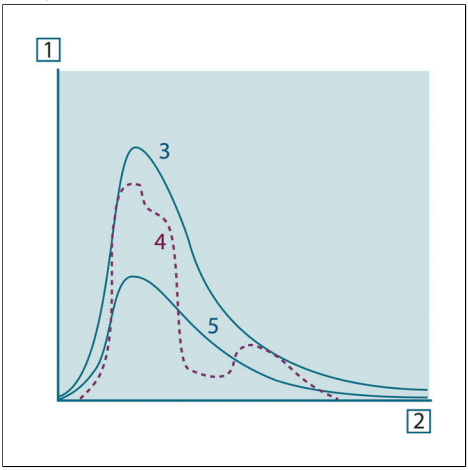

Figure 30.8 Spectral radiant emittance of three types of radiators. **1:** Spectral radiant emittance; **2:** Wavelength; **3:** Blackbody; **4:** Selective radiator; **5:** Graybody.

10327303;a4

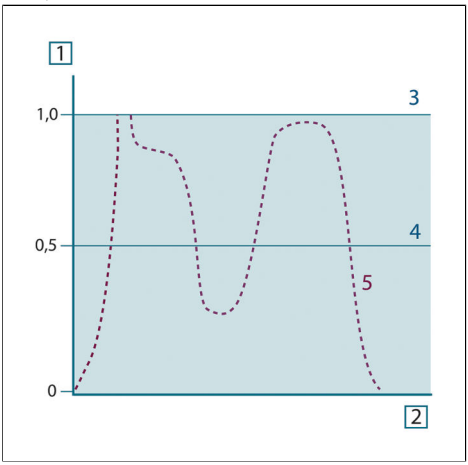

Figure 30.9 Spectral emissivity of three types of radiators. **1:** Spectral emissivity; **2:** Wavelength; **3:** Blackbody; **4:** Graybody; **5:** Selective radiator.

30.4 Infrared semi-transparent materials

Consider now a non-metallic, semi-transparent body – let us say, in the form of a thick flat plate of plastic material. When the plate is heated, radiation generated within its volume must work its way toward the surfaces through the material in which it is partially absorbed. Moreover, when it arrives at the surface, some of it is reflected back into the interior. The back-reflected radiation is again partially absorbed, but

actoolsupply.com

actoolsupply.com

some of it arrives at the other surface, through which most of it escapes; part of it is reflected back again. Although the progressive reflections become weaker and weaker they must all be added up when the total emittance of the plate is sought. When the resulting geometrical series is summed, the effective emissivity of a semi-transparent plate is obtained as:

$$\varepsilon_\lambda = \frac{(1-\rho_\lambda)(1-\tau_\lambda)}{1-\rho_\lambda\tau_\lambda}$$

When the plate becomes opaque this formula is reduced to the single formula:

$$\varepsilon_\lambda = 1-\rho_\lambda$$

This last relation is a particularly convenient one, because it is often easier to measure reflectance than to measure emissivity directly.

actoolsupply.com

actoolsupply.com

31 The measurement formula

As already mentioned, when viewing an object, the camera receives radiation not only from the object itself. It also collects radiation from the surroundings reflected via the object surface. Both these radiation contributions become attenuated to some extent by the atmosphere in the measurement path. To this comes a third radiation contribution from the atmosphere itself.

This description of the measurement situation, as illustrated in the figure below, is so far a fairly true description of the real conditions. What has been neglected could for instance be sun light scattering in the atmosphere or stray radiation from intense radiation sources outside the field of view. Such disturbances are difficult to quantify, however, in most cases they are fortunately small enough to be neglected. In case they are not negligible, the measurement configuration is likely to be such that the risk for disturbance is obvious, at least to a trained operator. It is then his responsibility to modify the measurement situation to avoid the disturbance e.g. by changing the viewing direction, shielding off intense radiation sources etc.

Accepting the description above, we can use the figure below to derive a formula for the calculation of the object temperature from the calibrated camera output.

10400503;a1

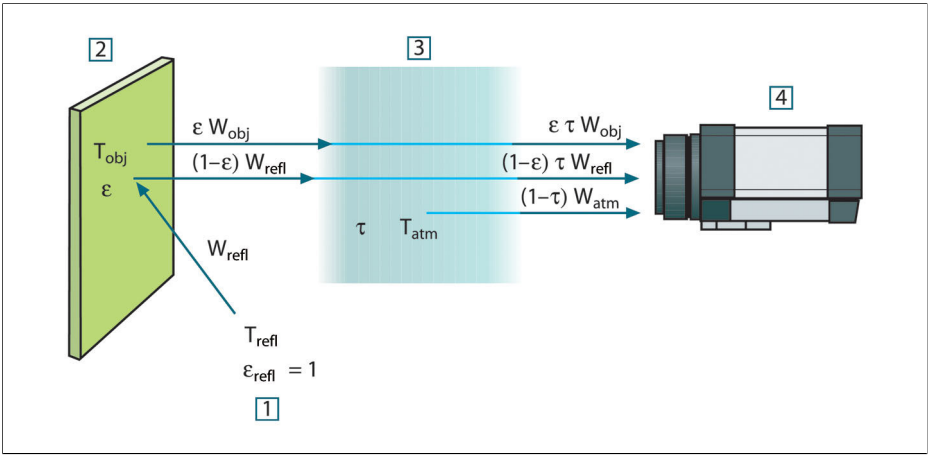

Figure 31.1 A schematic representation of the general thermographic measurement situation.**1:** Surroundings; **2:** Object; **3:** Atmosphere; **4:** Camera

Assume that the received radiation power W from a blackbody source of temperature T_{source} on short distance generates a camera output signal U_{source} that is proportional to the power input (power linear camera). We can then write (Equation 1):

actoolsupply.com

actoolsupply.com

$$U_{source} = CW(T_{source})$$

or, with simplified notation:

$$U_{source} = CW_{source}$$

where C is a constant.

Should the source be a graybody with emittance ε, the received radiation would consequently be εW_{source}.

We are now ready to write the three collected radiation power terms:

1 – Emission from the object = $\varepsilon\tau W_{obj}$, where ε is the emittance of the object and τ is the transmittance of the atmosphere. The object temperature is T_{obj}.

2 – Reflected emission from ambient sources = $(1 - \varepsilon)\tau W_{refl}$, where (1 – ε) is the reflectance of the object. The ambient sources have the temperature T_{refl}.

It has here been assumed that the temperature T_{refl} is the same for all emitting surfaces within the halfsphere seen from a point on the object surface. This is of course sometimes a simplification of the true situation. It is, however, a necessary simplification in order to derive a workable formula, and T_{refl} can – at least theoretically – be given a value that represents an efficient temperature of a complex surrounding.

Note also that we have assumed that the emittance for the surroundings = 1. This is correct in accordance with Kirchhoff's law: All radiation impinging on the surrounding surfaces will eventually be absorbed by the same surfaces. Thus the emittance = 1. (Note though that the latest discussion requires the complete sphere around the object to be considered.)

3 – Emission from the atmosphere = $(1 - \tau)\tau W_{atm}$, where (1 – τ) is the emittance of the atmosphere. The temperature of the atmosphere is T_{atm}.

The total received radiation power can now be written (Equation 2):

$$W_{tot} = \varepsilon\tau W_{obj} + (1 - \varepsilon)\tau W_{refl} + (1 - \tau)W_{atm}$$

We multiply each term by the constant C of Equation 1 and replace the CW products by the corresponding U according to the same equation, and get (Equation 3):

$$U_{tot} = \varepsilon\tau U_{obj} + (1 - \varepsilon)\tau U_{refl} + (1 - \tau)U_{atm}$$

Solve Equation 3 for U_{obj} (Equation 4):

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

$$U_{obj} = \frac{1}{\varepsilon\tau}U_{tot} - \frac{1-\varepsilon}{\varepsilon}U_{refl} - \frac{1-\tau}{\varepsilon\tau}U_{atm}$$

This is the general measurement formula used in all the FLIR Systems thermographic equipment. The voltages of the formula are:

Figure 31.2 Voltages

U_{obj}	Calculated camera output voltage for a blackbody of temperature T_{obj} i.e. a voltage that can be directly converted into true requested object temperature.
U_{tot}	Measured camera output voltage for the actual case.
U_{refl}	Theoretical camera output voltage for a blackbody of temperature T_{refl} according to the calibration.
U_{atm}	Theoretical camera output voltage for a blackbody of temperature T_{atm} according to the calibration.

The operator has to supply a number of parameter values for the calculation:

- the object emittance ε,
- the relative humidity,
- T_{atm}
- object distance (D_{obj})
- the (effective) temperature of the object surroundings, or the reflected ambient temperature T_{refl}, and
- the temperature of the atmosphere T_{atm}

This task could sometimes be a heavy burden for the operator since there are normally no easy ways to find accurate values of emittance and atmospheric transmittance for the actual case. The two temperatures are normally less of a problem provided the surroundings do not contain large and intense radiation sources.

A natural question in this connection is: How important is it to know the right values of these parameters? It could though be of interest to get a feeling for this problem already here by looking into some different measurement cases and compare the relative magnitudes of the three radiation terms. This will give indications about when it is important to use correct values of which parameters.

The figures below illustrates the relative magnitudes of the three radiation contributions for three different object temperatures, two emittances, and two spectral ranges: SW and LW. Remaining parameters have the following fixed values:

- $\tau = 0.88$
- T_{refl} = +20°C (+68°F)
- T_{atm} = +20°C (+68°F)

actoolsupply.com

actoolsupply.com

It is obvious that measurement of low object temperatures are more critical than measuring high temperatures since the 'disturbing' radiation sources are relatively much stronger in the first case. Should also the object emittance be low, the situation would be still more difficult.

We have finally to answer a question about the importance of being allowed to use the calibration curve above the highest calibration point, what we call extrapolation. Imagine that we in a certain case measure $U_{tot} = 4.5$ volts. The highest calibration point for the camera was in the order of 4.1 volts, a value unknown to the operator. Thus, even if the object happened to be a blackbody, i.e. $U_{obj} = U_{tot}$, we are actually performing extrapolation of the calibration curve when converting 4.5 volts into temperature.

Let us now assume that the object is not black, it has an emittance of 0.75, and the transmittance is 0.92. We also assume that the two second terms of Equation 4 amount to 0.5 volts together. Computation of U_{obj} by means of Equation 4 then results in $U_{obj} = 4.5 / 0.75 / 0.92 – 0.5 = 6.0$. This is a rather extreme extrapolation, particularly when considering that the video amplifier might limit the output to 5 volts! Note, though, that the application of the calibration curve is a theoretical procedure where no electronic or other limitations exist. We trust that if there had been no signal limitations in the camera, and if it had been calibrated far beyond 5 volts, the resulting curve would have been very much the same as our real curve extrapolated beyond 4.1 volts, provided the calibration algorithm is based on radiation physics, like the FLIR Systems algorithm. Of course there must be a limit to such extrapolations.

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

10400603;a2

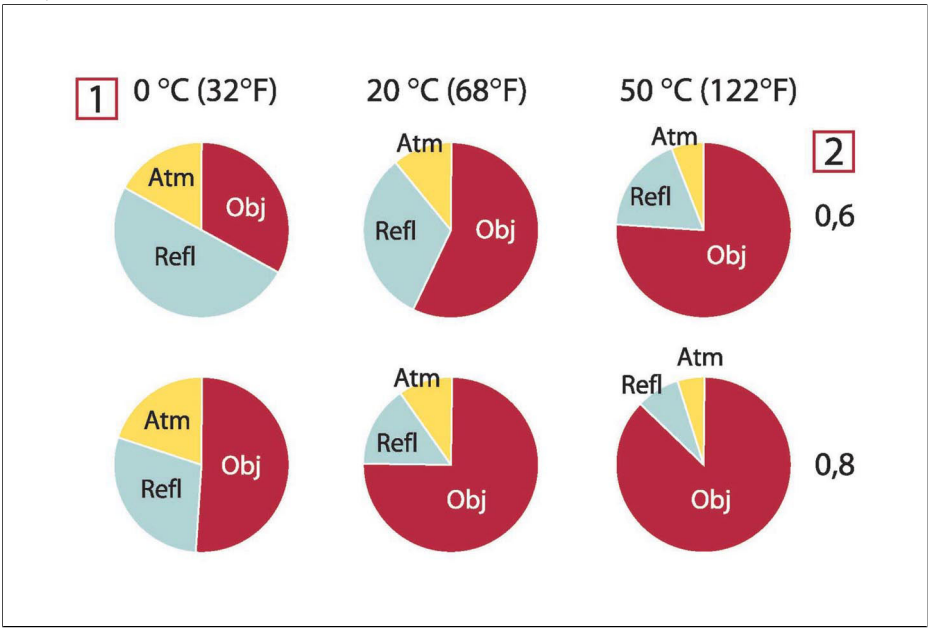

Figure 31.3 Relative magnitudes of radiation sources under varying measurement conditions (SW camera). **1:** Object temperature; **2:** Emittance; **Obj:** Object radiation; **Refl:** Reflected radiation; **Atm:** atmosphere radiation. Fixed parameters: $\tau = 0.88$; $T_{refl} = 20°C$ (+68°F); $T_{atm} = 20°C$ (+68°F).

actoolsupply.com

actoolsupply.com

10400703;a2

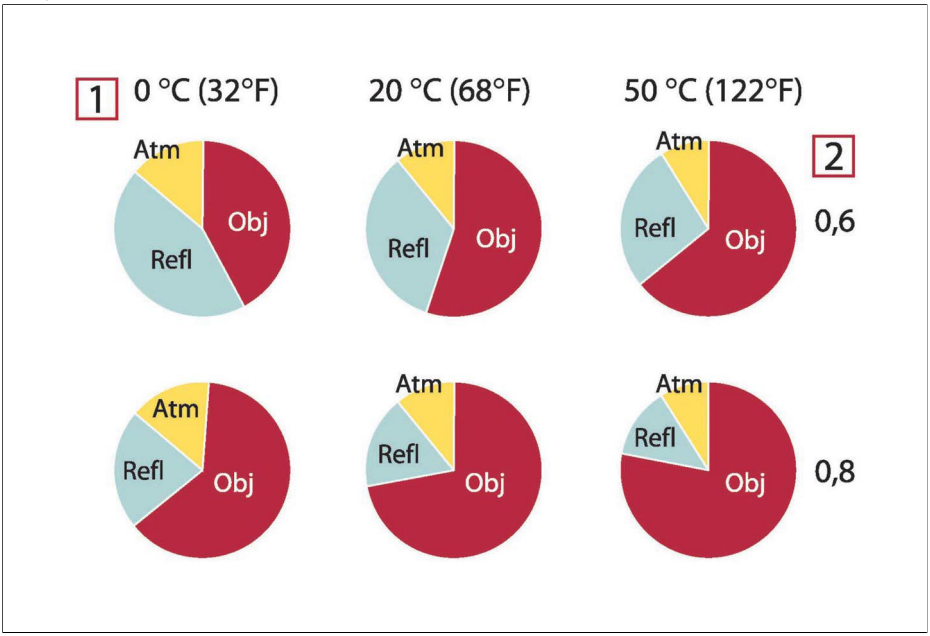

Figure 31.4 Relative magnitudes of radiation sources under varying measurement conditions (LW camera). **1:** Object temperature; **2:** Emittance; **Obj:** Object radiation; **Refl:** Reflected radiation; **Atm:** atmosphere radiation. Fixed parameters: $\tau = 0.88$; $T_{refl} = 20°C$ (+68°F); $T_{atm} = 20°C$ (+68°F).

actoolsupply.com

actoolsupply.com

32 Emissivity tables

This section presents a compilation of emissivity data from the infrared literature and measurements made by FLIR Systems.

32.1 References

1	Mikaél A. Bramson: *Infrared Radiation, A Handbook for Applications*, Plenum press, N.Y.
2	William L. Wolfe, George J. Zissis: *The Infrared Handbook*, Office of Naval Research, Department of Navy, Washington, D.C.
3	Madding, R. P.: *Thermographic Instruments and systems*. Madison, Wisconsin: University of Wisconsin – Extension, Department of Engineering and Applied Science.
4	William L. Wolfe: *Handbook of Military Infrared Technology*, Office of Naval Research, Department of Navy, Washington, D.C.
5	Jones, Smith, Probert: *External thermography of buildings...,* Proc. of the Society of Photo-Optical Instrumentation Engineers, vol.110, Industrial and Civil Applications of Infrared Technology, June 1977 London.
6	Paljak, Pettersson: *Thermography of Buildings*, Swedish Building Research Institute, Stockholm 1972.
7	Vlcek, J: *Determination of emissivity with imaging radiometers and some emissivities at λ = 5 µm.* Photogrammetric Engineering and Remote Sensing.
8	Kern: *Evaluation of infrared emission of clouds and ground as measured by weather satellites*, Defence Documentation Center, AD 617 417.
9	Öhman, Claes: *Emittansmätningar med AGEMA E-Box*. Teknisk rapport, AGEMA 1999. (Emittance measurements using AGEMA E-Box. Technical report, AGEMA 1999.)
10	Matteï, S., Tang-Kwor, E: *Emissivity measurements for Nextel Velvet coating 811-21 between –36°C AND 82°C.*
11	Lohrengel & Todtenhaupt (1996)
12	ITC Technical publication 32.
13	ITC Technical publication 29.

32.2 Important note about the emissivity tables

The type of camera that has been used when compiling the emissivity data is specified in column 4. The values should be regarded as recommendations only and used with caution.

actoolsupply.com

actoolsupply.com

32.3 Tables

Figure 32.1 1: Material; **2:** Specification; **3:** Temperature in °C; **4:** Spectrum (**T:** Total spectrum; **SW:** 2–5 μm; **LW:** 8–14 μm, **LLW:** 6.5–20 μm); **5:** Emissivity: **6:** Reference to literature source above

1	2	3	4	5	6
3M type 35	Vinyl electrical tape (several colors)	< 80	LW	Ca. 0.96	13
3M type 88	Black vinyl electrical tape	< 105	LW	Ca. 0.96	13
3M type 88	Black vinyl electrical tape	< 105	MW	< 0.96	13
3M type Super 33+	Black vinyl electrical tape	< 80	LW	Ca. 0.96	13
Aluminum	anodized, black, dull	70	LW	0.95	9
Aluminum	anodized, black, dull	70	SW	0.67	9
Aluminum	anodized, light gray, dull	70	LW	0.97	9
Aluminum	anodized, light gray, dull	70	SW	0.61	9
Aluminum	anodized sheet	100	T	0.55	2
Aluminum	as received, plate	100	T	0.09	4
Aluminum	as received, sheet	100	T	0.09	2
Aluminum	cast, blast cleaned	70	LW	0.46	9
Aluminum	cast, blast cleaned	70	SW	0.47	9
Aluminum	dipped in HNO_3, plate	100	T	0.05	4
Aluminum	foil	27	3 μm	0.09	3
Aluminum	foil	27	10 μm	0.04	3
Aluminum	oxidized, strongly	50–500	T	0.2–0.3	1
Aluminum	polished	50–100	T	0.04–0.06	1
Aluminum	polished, sheet	100	T	0.05	2
Aluminum	polished plate	100	T	0.05	4

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

1	2	3	4	5	6
Aluminum	roughened	27	3 µm	0.28	3
Aluminum	roughened	27	10 µm	0.18	3
Aluminum	rough surface	20–50	T	0.06–0.07	1
Aluminum	sheet, 4 samples differently scratched	70	LW	0.03–0.06	9
Aluminum	sheet, 4 samples differently scratched	70	SW	0.05–0.08	9
Aluminum	vacuum deposited	20	T	0.04	2
Aluminum	weathered, heavily	17	SW	0.83–0.94	5
Aluminum bronze		20	T	0.60	1
Aluminum hydroxide	powder		T	0.28	1
Aluminum oxide	activated, powder		T	0.46	1
Aluminum oxide	pure, powder (alumina)		T	0.16	1
Asbestos	board	20	T	0.96	1
Asbestos	fabric		T	0.78	1
Asbestos	floor tile	35	SW	0.94	7
Asbestos	paper	40–400	T	0.93–0.95	1
Asbestos	powder		T	0.40–0.60	1
Asbestos	slate	20	T	0.96	1
Asphalt paving		4	LLW	0.967	8
Brass	dull, tarnished	20–350	T	0.22	1
Brass	oxidized	70	SW	0.04–0.09	9
Brass	oxidized	70	LW	0.03–0.07	9
Brass	oxidized	100	T	0.61	2
Brass	oxidized at 600°C	200–600	T	0.59–0.61	1
Brass	polished	200	T	0.03	1
Brass	polished, highly	100	T	0.03	2

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Brass	rubbed with 80-grit emery	20	T	0.20	2
Brass	sheet, rolled	20	T	0.06	1
Brass	sheet, worked with emery	20	T	0.2	1
Brick	alumina	17	SW	0.68	5
Brick	common	17	SW	0.86–0.81	5
Brick	Dinas silica, glazed, rough	1100	T	0.85	1
Brick	Dinas silica, refractory	1000	T	0.66	1
Brick	Dinas silica, unglazed, rough	1000	T	0.80	1
Brick	firebrick	17	SW	0.68	5
Brick	fireclay	20	T	0.85	1
Brick	fireclay	1000	T	0.75	1
Brick	fireclay	1200	T	0.59	1
Brick	masonry	35	SW	0.94	7
Brick	masonry, plastered	20	T	0.94	1
Brick	red, common	20	T	0.93	2
Brick	red, rough	20	T	0.88–0.93	1
Brick	refractory, corundum	1000	T	0.46	1
Brick	refractory, magnesite	1000–1300	T	0.38	1
Brick	refractory, strongly radiating	500–1000	T	0.8–0.9	1
Brick	refractory, weakly radiating	500–1000	T	0.65–0.75	1
Brick	silica, 95% SiO_2	1230	T	0.66	1
Brick	sillimanite, 33% SiO_2, 64% Al_2O_3	1500	T	0.29	1

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Brick	waterproof	17	SW	0.87	5
Bronze	phosphor bronze	70	LW	0.06	9
Bronze	phosphor bronze	70	SW	0.08	9
Bronze	polished	50	T	0.1	1
Bronze	porous, rough	50–150	T	0.55	1
Bronze	powder		T	0.76–0.80	1
Carbon	candle soot	20	T	0.95	2
Carbon	charcoal powder		T	0.96	1
Carbon	graphite, filed surface	20	T	0.98	2
Carbon	graphite powder		T	0.97	1
Carbon	lampblack	20–400	T	0.95–0.97	1
Chipboard	untreated	20	SW	0.90	6
Chromium	polished	50	T	0.10	1
Chromium	polished	500–1000	T	0.28–0.38	1
Clay	fired	70	T	0.91	1
Cloth	black	20	T	0.98	1
Concrete		20	T	0.92	2
Concrete	dry	36	SW	0.95	7
Concrete	rough	17	SW	0.97	5
Concrete	walkway	5	LLW	0.974	8
Copper	commercial, burnished	20	T	0.07	1
Copper	electrolytic, carefully polished	80	T	0.018	1
Copper	electrolytic, polished	–34	T	0.006	4
Copper	molten	1100–1300	T	0.13–0.15	1
Copper	oxidized	50	T	0.6–0.7	1
Copper	oxidized, black	27	T	0.78	4

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Copper	oxidized, heavily	20	T	0.78	2
Copper	oxidized to blackness		T	0.88	1
Copper	polished	50–100	T	0.02	1
Copper	polished	100	T	0.03	2
Copper	polished, commercial	27	T	0.03	4
Copper	polished, mechanical	22	T	0.015	4
Copper	pure, carefully prepared surface	22	T	0.008	4
Copper	scraped	27	T	0.07	4
Copper dioxide	powder		T	0.84	1
Copper oxide	red, powder		T	0.70	1
Ebonite			T	0.89	1
Emery	coarse	80	T	0.85	1
Enamel		20	T	0.9	1
Enamel	lacquer	20	T	0.85–0.95	1
Fiber board	hard, untreated	20	SW	0.85	6
Fiber board	masonite	70	LW	0.88	9
Fiber board	masonite	70	SW	0.75	9
Fiber board	particle board	70	LW	0.89	9
Fiber board	particle board	70	SW	0.77	9
Fiber board	porous, untreated	20	SW	0.85	6
Gold	polished	130	T	0.018	1
Gold	polished, carefully	200–600	T	0.02–0.03	1
Gold	polished, highly	100	T	0.02	2
Granite	polished	20	LLW	0.849	8
Granite	rough	21	LLW	0.879	8
Granite	rough, 4 different samples	70	LW	0.77–0.87	9

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

1	2	3	4	5	6
Granite	rough, 4 different samples	70	SW	0.95–0.97	9
Gypsum		20	T	0.8–0.9	1
Ice: See Water					
Iron, cast	casting	50	T	0.81	1
Iron, cast	ingots	1000	T	0.95	1
Iron, cast	liquid	1300	T	0.28	1
Iron, cast	machined	800–1000	T	0.60–0.70	1
Iron, cast	oxidized	38	T	0.63	4
Iron, cast	oxidized	100	T	0.64	2
Iron, cast	oxidized	260	T	0.66	4
Iron, cast	oxidized	538	T	0.76	4
Iron, cast	oxidized at 600°C	200–600	T	0.64–0.78	1
Iron, cast	polished	38	T	0.21	4
Iron, cast	polished	40	T	0.21	2
Iron, cast	polished	200	T	0.21	1
Iron, cast	unworked	900–1100	T	0.87–0.95	1
Iron and steel	cold rolled	70	LW	0.09	9
Iron and steel	cold rolled	70	SW	0.20	9
Iron and steel	covered with red rust	20	T	0.61–0.85	1
Iron and steel	electrolytic	22	T	0.05	4
Iron and steel	electrolytic	100	T	0.05	4
Iron and steel	electrolytic	260	T	0.07	4
Iron and steel	electrolytic, carefully polished	175–225	T	0.05–0.06	1
Iron and steel	freshly worked with emery	20	T	0.24	1
Iron and steel	ground sheet	950–1100	T	0.55–0.61	1
Iron and steel	heavily rusted sheet	20	T	0.69	2

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Iron and steel	hot rolled	20	T	0.77	1
Iron and steel	hot rolled	130	T	0.60	1
Iron and steel	oxidized	100	T	0.74	1
Iron and steel	oxidized	100	T	0.74	4
Iron and steel	oxidized	125–525	T	0.78–0.82	1
Iron and steel	oxidized	200	T	0.79	2
Iron and steel	oxidized	1227	T	0.89	4
Iron and steel	oxidized	200–600	T	0.80	1
Iron and steel	oxidized strongly	50	T	0.88	1
Iron and steel	oxidized strongly	500	T	0.98	1
Iron and steel	polished	100	T	0.07	2
Iron and steel	polished	400–1000	T	0.14–0.38	1
Iron and steel	polished sheet	750–1050	T	0.52–0.56	1
Iron and steel	rolled, freshly	20	T	0.24	1
Iron and steel	rolled sheet	50	T	0.56	1
Iron and steel	rough, plane surface	50	T	0.95–0.98	1
Iron and steel	rusted, heavily	17	SW	0.96	5
Iron and steel	rusted red, sheet	22	T	0.69	4
Iron and steel	rusty, red	20	T	0.69	1
Iron and steel	shiny, etched	150	T	0.16	1
Iron and steel	shiny oxide layer, sheet,	20	T	0.82	1
Iron and steel	wrought, carefully polished	40–250	T	0.28	1
Iron galvanized	heavily oxidized	70	LW	0.85	9
Iron galvanized	heavily oxidized	70	SW	0.64	9
Iron galvanized	sheet	92	T	0.07	4
Iron galvanized	sheet, burnished	30	T	0.23	1
Iron galvanized	sheet, oxidized	20	T	0.28	1

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Iron tinned	sheet	24	T	0.064	4
Krylon Ultra-flat black 1602	Flat black	Room temperature up to 175	LW	Ca. 0.96	12
Krylon Ultra-flat black 1602	Flat black	Room temperature up to 175	MW	Ca. 0.97	12
Lacquer	3 colors sprayed on Aluminum	70	LW	0.92–0.94	9
Lacquer	3 colors sprayed on Aluminum	70	SW	0.50–0.53	9
Lacquer	Aluminum on rough surface	20	T	0.4	1
Lacquer	bakelite	80	T	0.83	1
Lacquer	black, dull	40–100	T	0.96–0.98	1
Lacquer	black, matte	100	T	0.97	2
Lacquer	black, shiny, sprayed on iron	20	T	0.87	1
Lacquer	heat–resistant	100	T	0.92	1
Lacquer	white	40–100	T	0.8–0.95	1
Lacquer	white	100	T	0.92	2
Lead	oxidized, gray	20	T	0.28	1
Lead	oxidized, gray	22	T	0.28	4
Lead	oxidized at 200°C	200	T	0.63	1
Lead	shiny	250	T	0.08	1
Lead	unoxidized, polished	100	T	0.05	4
Lead red		100	T	0.93	4
Lead red, powder		100	T	0.93	1
Leather	tanned		T	0.75–0.80	1
Lime			T	0.3–0.4	1
Magnesium		22	T	0.07	4
Magnesium		260	T	0.13	4

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Magnesium		538	T	0.18	4
Magnesium	polished	20	T	0.07	2
Magnesium powder			T	0.86	1
Molybdenum		600–1000	T	0.08–0.13	1
Molybdenum		1500–2200	T	0.19–0.26	1
Molybdenum	filament	700–2500	T	0.1–0.3	1
Mortar		17	SW	0.87	5
Mortar	dry	36	SW	0.94	7
Nextel Velvet 811-21 Black	Flat black	–60–150	LW	> 0.97	10 and 11
Nichrome	rolled	700	T	0.25	1
Nichrome	sandblasted	700	T	0.70	1
Nichrome	wire, clean	50	T	0.65	1
Nichrome	wire, clean	500–1000	T	0.71–0.79	1
Nichrome	wire, oxidized	50–500	T	0.95–0.98	1
Nickel	bright matte	122	T	0.041	4
Nickel	commercially pure, polished	100	T	0.045	1
Nickel	commercially pure, polished	200–400	T	0.07–0.09	1
Nickel	electrolytic	22	T	0.04	4
Nickel	electrolytic	38	T	0.06	4
Nickel	electrolytic	260	T	0.07	4
Nickel	electrolytic	538	T	0.10	4
Nickel	electroplated, polished	20	T	0.05	2
Nickel	electroplated on iron, polished	22	T	0.045	4
Nickel	electroplated on iron, unpolished	20	T	0.11–0.40	1

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

1	2	3	4	5	6
Nickel	electroplated on iron, unpolished	22	T	0.11	4
Nickel	oxidized	200	T	0.37	2
Nickel	oxidized	227	T	0.37	4
Nickel	oxidized	1227	T	0.85	4
Nickel	oxidized at 600°C	200–600	T	0.37–0.48	1
Nickel	polished	122	T	0.045	4
Nickel	wire	200–1000	T	0.1–0.2	1
Nickel oxide		500–650	T	0.52–0.59	1
Nickel oxide		1000–1250	T	0.75–0.86	1
Oil, lubricating	0.025 mm film	20	T	0.27	2
Oil, lubricating	0.050 mm film	20	T	0.46	2
Oil, lubricating	0.125 mm film	20	T	0.72	2
Oil, lubricating	film on Ni base: Ni base only	20	T	0.05	2
Oil, lubricating	thick coating	20	T	0.82	2
Paint	8 different colors and qualities	70	LW	0.92–0.94	9
Paint	8 different colors and qualities	70	SW	0.88–0.96	9
Paint	Aluminum, various ages	50–100	T	0.27–0.67	1
Paint	cadmium yellow		T	0.28–0.33	1
Paint	chrome green		T	0.65–0.70	1
Paint	cobalt blue		T	0.7–0.8	1
Paint	oil	17	SW	0.87	5
Paint	oil, black flat	20	SW	0.94	6
Paint	oil, black gloss	20	SW	0.92	6
Paint	oil, gray flat	20	SW	0.97	6
Paint	oil, gray gloss	20	SW	0.96	6
Paint	oil, various colors	100	T	0.92–0.96	1

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Paint	oil based, average of 16 colors	100	T	0.94	2
Paint	plastic, black	20	SW	0.95	6
Paint	plastic, white	20	SW	0.84	6
Paper	4 different colors	70	LW	0.92–0.94	9
Paper	4 different colors	70	SW	0.68–0.74	9
Paper	black		T	0.90	1
Paper	black, dull		T	0.94	1
Paper	black, dull	70	LW	0.89	9
Paper	black, dull	70	SW	0.86	9
Paper	blue, dark		T	0.84	1
Paper	coated with black lacquer		T	0.93	1
Paper	green		T	0.85	1
Paper	red		T	0.76	1
Paper	white	20	T	0.7–0.9	1
Paper	white, 3 different glosses	70	LW	0.88–0.90	9
Paper	white, 3 different glosses	70	SW	0.76–0.78	9
Paper	white bond	20	T	0.93	2
Paper	yellow		T	0.72	1
Plaster		17	SW	0.86	5
Plaster	plasterboard, untreated	20	SW	0.90	6
Plaster	rough coat	20	T	0.91	2
Plastic	glass fibre laminate (printed circ. board)	70	LW	0.91	9
Plastic	glass fibre laminate (printed circ. board)	70	SW	0.94	9

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Plastic	polyurethane isolation board	70	LW	0.55	9
Plastic	polyurethane isolation board	70	SW	0.29	9
Plastic	PVC, plastic floor, dull, structured	70	LW	0.93	9
Plastic	PVC, plastic floor, dull, structured	70	SW	0.94	9
Platinum		17	T	0.016	4
Platinum		22	T	0.03	4
Platinum		100	T	0.05	4
Platinum		260	T	0.06	4
Platinum		538	T	0.10	4
Platinum		1000–1500	T	0.14–0.18	1
Platinum		1094	T	0.18	4
Platinum	pure, polished	200–600	T	0.05–0.10	1
Platinum	ribbon	900–1100	T	0.12–0.17	1
Platinum	wire	50–200	T	0.06–0.07	1
Platinum	wire	500–1000	T	0.10–0.16	1
Platinum	wire	1400	T	0.18	1
Porcelain	glazed	20	T	0.92	1
Porcelain	white, shiny		T	0.70–0.75	1
Rubber	hard	20	T	0.95	1
Rubber	soft, gray, rough	20	T	0.95	1
Sand			T	0.60	1
Sand		20	T	0.90	2
Sandstone	polished	19	LLW	0.909	8
Sandstone	rough	19	LLW	0.935	8
Silver	polished	100	T	0.03	2
Silver	pure, polished	200–600	T	0.02–0.03	1

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Skin	human	32	T	0.98	2
Slag	boiler	0–100	T	0.97–0.93	1
Slag	boiler	200–500	T	0.89–0.78	1
Slag	boiler	600–1200	T	0.76–0.70	1
Slag	boiler	1400–1800	T	0.69–0.67	1
Snow: See Water					
Soil	dry	20	T	0.92	2
Soil	saturated with water	20	T	0.95	2
Stainless steel	alloy, 8% Ni, 18% Cr	500	T	0.35	1
Stainless steel	rolled	700	T	0.45	1
Stainless steel	sandblasted	700	T	0.70	1
Stainless steel	sheet, polished	70	LW	0.14	9
Stainless steel	sheet, polished	70	SW	0.18	9
Stainless steel	sheet, untreated, somewhat scratched	70	LW	0.28	9
Stainless steel	sheet, untreated, somewhat scratched	70	SW	0.30	9
Stainless steel	type 18-8, buffed	20	T	0.16	2
Stainless steel	type 18-8, oxidized at 800°C	60	T	0.85	2
Stucco	rough, lime	10–90	T	0.91	1
Styrofoam	insulation	37	SW	0.60	7
Tar			T	0.79–0.84	1
Tar	paper	20	T	0.91–0.93	1
Tile	glazed	17	SW	0.94	5
Tin	burnished	20–50	T	0.04–0.06	1
Tin	tin–plated sheet iron	100	T	0.07	2

actoolsupply.com

actoolsupply.com

AC TOOL SUPPLY.COM 877-207-1244 aikencolon.com

1	2	3	4	5	6
Titanium	oxidized at 540°C	200	T	0.40	1
Titanium	oxidized at 540°C	500	T	0.50	1
Titanium	oxidized at 540°C	1000	T	0.60	1
Titanium	polished	200	T	0.15	1
Titanium	polished	500	T	0.20	1
Titanium	polished	1000	T	0.36	1
Tungsten		200	T	0.05	1
Tungsten		600–1000	T	0.1–0.16	1
Tungsten		1500–2200	T	0.24–0.31	1
Tungsten	filament	3300	T	0.39	1
Varnish	flat	20	SW	0.93	6
Varnish	on oak parquet floor	70	LW	0.90–0.93	9
Varnish	on oak parquet floor	70	SW	0.90	9
Wallpaper	slight pattern, light gray	20	SW	0.85	6
Wallpaper	slight pattern, red	20	SW	0.90	6
Water	distilled	20	T	0.96	2
Water	frost crystals	–10	T	0.98	2
Water	ice, covered with heavy frost	0	T	0.98	1
Water	ice, smooth	–10	T	0.96	2
Water	ice, smooth	0	T	0.97	1
Water	layer >0.1 mm thick	0–100	T	0.95–0.98	1
Water	snow		T	0.8	1
Water	snow	–10	T	0.85	2
Wood		17	SW	0.98	5
Wood		19	LLW	0.962	8
Wood	ground		T	0.5–0.7	1

actoolsupply.com

actoolsupply.com

1	2	3	4	5	6
Wood	pine, 4 different samples	70	LW	0.81–0.89	9
Wood	pine, 4 different samples	70	SW	0.67–0.75	9
Wood	planed	20	T	0.8–0.9	1
Wood	planed oak	20	T	0.90	2
Wood	planed oak	70	LW	0.88	9
Wood	planed oak	70	SW	0.77	9
Wood	plywood, smooth, dry	36	SW	0.82	7
Wood	plywood, untreated	20	SW	0.83	6
Wood	white, damp	20	T	0.7–0.8	1
Zinc	oxidized at 400°C	400	T	0.11	1
Zinc	oxidized surface	1000–1200	T	0.50–0.60	1
Zinc	polished	200–300	T	0.04–0.05	1
Zinc	sheet	50	T	0.20	1

actoolsupply.com

actoolsupply.com

A note on the technical production of this publication

This publication was produced using XML—the e*Xtensible Markup Language*. For more information about XML, please visit http://www.w3.org/XML/

A note on the typeface used in this publication

This publication was typeset using Swiss 721, which is Bitstream's pan-European version of the Helvetica™ typeface. Helvetica™ was designed by Max Miedinger (1910–1980).

List of effective files

20235103.xml a24
20235203.xml a21
20235303.xml a19
20236703.xml a57
20237103.xml a10
20238503.xml a9
20238703.xml b8
20250403.xml a21
20254903.xml a75a3
20257003.xml a40
20257103.xml a17
20257303.xml a35
20279803.xml a8
20281003.xml a1
20283703.xml a11
20283803.xml a5
20283903.xml a5
20284003.xml a12
20284103.xml a13
20284203.xml a11
20284303.xml a8
20284403.xml a10
20284503.xml a9
20284703.xml a8
20284803.xml a5
20284903.xml a20
20285103.xml a6
20285203.xml a4
20287303.xml a9
20288603.xml a4
20288703.xml a5
20292403.xml a5
20294903.xml a5
20295003.xml a14
20295303.xml a2
R110.rcp a9
config.xml a5

actoolsupply.com

AC Tool Supply.com
877-207-1244
aikencolon.com